



Alaska Department of Transportation and Public Facilities

Alaska Test Methods Manual

Revised June 15, 2010

Preface

This manual provides a compilation of approved Test Methods, Forms and Standard Practices to be used to test materials on Alaska Department of Transportation & Public Facilities (DOT&PF) projects.

Most of these testing procedures follow two nationally recognized standards; American Society for Testing and Materials (ASTM), and the American Association of State Highway and Transportation Officials (AASHTO). Modifications to these standards are in recognition of the necessity of adjusting test requirements to meet local demands and/or naturally occurring materials.

This manual also includes Field Operating Procedures (FOPs) for existing AASHTO test methods. These procedures are developed and maintained by the Western Alliance for Quality in Transportation Construction (WAQTC). The FOPs select options and provide concise directions in the use of the AASHTO methods.

In addition, this manual includes WAQTC test methods that are not covered by AASHTO or ASTM. These methods have been submitted to AASHTO for adoption. Other procedures were developed by the Alaska DOT&PF to address specific needs in the State of Alaska that are not adequately covered in AASHTO, ASTM or WAQTC.

The Appendix contains standardized practices to be used by all DOT&PF regional and/or field laboratories including consultant fixed and field laboratories.

Any additions, deletions or revisions to these procedures shall be made through the office of the Chief Engineer.

Acknowledgement

Design and Engineering Services, Statewide Materials is indebted to the following organizations for use of, or reference to, portions of their publications.

The American Association of State Highway and Transportation Officials
The American Society for Testing and Materials

Appreciation is also extended to Laboratory and Construction personnel from each Region for their dedication and patience in seeing this task to completion.

Seventh Edition Printing, April 15, 2010

List of Revisions for this edition:

1. TOC, All Descriptions are updated to exactly match the ATM and AASHTO titles. TP 61 is updated to: T 335. ATM 520 is deleted in TOC and Manual due to lack of use. Addendum added to T 85 noted in TOC.
2. WAQTC FOPs in general will have numerical examples of computations removed. These will be maintained in the WAQTC Training Manuals.
3. 202 – WAQTC FOP for AASHTO T 255/T 265 – Minor editorial changes and Addendum:
1. *When drying aggregates, drying overnight shall be sufficient to reach constant mass.*
4. 207 - WAQTC FOP for AASHTO T 99/T 180. Minor editorial changes.
5. 212 – ATM 212 has minor editorial changes.
6. 213 - WAQTC FOP for AASHTO T 310 has minor editorial changes.
7. 213 - WAQTC FOP for AASHTO T 224 has minor editorial changes and a new Addendum item that states: *When results are used for acceptance, the Specific Gravity shall be determined.*
8. 301 - WAQTC FOP for AASHTO T 2 has minor editorial changes and Addendum item 1 is deleted. *New Addendum item added:*
As an alternate to stockpile sampling Method A, use a loader to deposit a cross section of the stockpile in a pile, mix and distribute into a flattened miniature stockpile or pad 12” to 18” thick. Sample as indicated in Roadway Method B.
9. 301 - WAQTC FOP for AASHTO T 248 all mixing of samples in method B now require 4 times turning over the sample. The rest are minor editorial changes. Addendum 2 is reworded to read: *AASHTO T 248 Method C may be used.*
10. 304 – WAQTC FOR AASHTO T 27/T 11. Minor edits and the equation for overload determination is updated to give grams. Table 1 is corrected. Addendum 4 is added that reads:
4. For calculating Fineness Modulus, subtract reported percent passing from 100 to determine percent retained.
11. 305 – WAQTC FOP for AASHTO T 335 has minor editorial.
12. 307 – WAQTC FOP for AASHTO T 176 has minor editorial changes.
13. 308 – WAQTC FOP for AASHTO T 85 has minor editorial. Added addendum for averaging portions of sample run separately.
14. 309 - *Relative Standard Density of Soils by the Control Strip Method* is added as a new method.
15. 312 – Nordic Abrasion Value of Coarse Aggregate has minor editorial changes.
16. 401 - WAQTC FOP for AASHTO T 40. Addendum 2 states modified asphalt containers are the same as asphalt binder.
17. 402 - WAQTC FOP for AASHTO T 168 has minor editorial changes.
18. 403 - Sampling HMA – Has minor editorial changes.

Contents

Section 200 Earthwork

Title	Description	Section
ATM 201	Sticks and Roots Content of Aggregate and Soil	201
WAQTC FOP for AASHTO T 255/T 265	Moisture Content of Aggregate and Soils*	202
ATM 203	Organic Content of Soils	203
WAQTC FOP for AASHTO T 89	Determining the Liquid Limit of Soils	204
WAQTC FOP for AASHTO T 90	Determining the Plastic Limit and Plasticity Index of Soils	205
ATM 206	pH of Topsoil	206
WAQTC FOP for AASHTO T 99/ T 180	Moisture-Density Relations of Soils*	207
ATM 212	Determining the Standard Density of Coarse Granular Materials using the Vibratory Compactor	212
WAQTC FOP for AASHTO T 310	In-Place Density and Moisture Content of Soil and Soil-Aggregate by Nuclear Methods (Shallow Depth)*	213
WAQTC FOP for AASHTO T 224	Correction for Coarse Particles in the Soil Compaction Test*	214

Section 300 Bases and Aggregates

Title	Description	Section
WAQTC FOP for AASHTO T 2	Sampling of Aggregates*	301
WAQTC FOP for AASHTO T 248	Reducing Samples of Aggregate to Test Size*	303
WAQTC FOP for AASHTO T 27/T 11	Sieve Analysis of Fine and Coarse Aggregates *	304
WAQTC FOP for AASHTO 335	Determining the Percentage of Fracture in Coarse Aggregate	305
ATM 306	Determining the Percentage of Flat and Elongated Particles in Coarse Aggregate*	306
WAQTC FOP for AASHTO T 176	Plastic Fines in Graded Aggregates and Soils by Use of the Sand Equivalent Test	307
WAQTC FOP for AASHTO T 85	Specific Gravity and Absorption of Coarse Aggregate*	308
ATM 309	Relative Standard Density by the Control Strip Method	309
ATM 312	Nordic Abrasion Value of Coarse Aggregate	312
ATM 313	Degradation Value of Aggregates	313
ATM 314	Expansive Breakdown of Stone on Soaking in Ethylene Glycol	314

*This Test Method has an Addendum attached which has specific instructions for the use of the noted test method by the State of Alaska DOT&PF.

Section 400 Asphalt

Title	Description	Section
WAQTC FOP for AASHTO T 40	Sampling Bituminous Materials*	401
WAQTC FOP for AASHTO T 168	Sampling Bituminous Mixes*	402
ATM 403	Sampling Hot Mix Asphalt	403
WAQTC FOP for AASHTO R 47	Reducing Samples of Hot Mix Asphalt (HMA) to Testing Size*	404
ATM 405	Asphalt Cement Content of Hot Mix Asphalt by the Nuclear Method	405
WAQTC FOP for AASHTO T 308	Asphalt Binder Content of Hot Mix Asphalt (HMA) by Ignition Method*	406
WAQTC FOP for AASHTO T 329	Moisture Content of Hot Mix Asphalt (HMA) by Oven Method	407
WAQTC FOP for AASHTO T 30	Mechanical Analysis of Extracted Aggregate*	408
WAQTC FOP for AASHTO T 209	Theoretical Maximum Specific Gravity of Hot Mix Asphalt (HMA)*	409
WAQTC FOP for AASHTO T 166/T 275	Bulk Specific Gravity of Compacted Hot Mix Asphalt (HMA)*	410
WAQTC TM 8	In-Place Density of Bituminous Mixes using the Nuclear Moisture-Density Gauge*	411
ATM 412	Relative Standard Density by the Control Strip Method	412
WAQTC TM 11	Sampling Bituminous Material after Compaction (Obtaining Cores)*	413
ATM 414	Anti-Strip Requirements of Hot Mix Asphalt	414
ATM 417	Hot Mix Asphalt Design by the Marshall Method	417
ATM 419	Rutting Susceptibility using an Asphalt Pavement Analyzer	419

*This Test Method has an Addendum attached which has specific instructions for the use of the noted test method by the State of Alaska DOT&PF.

Section 500 Concrete

Title	Description	Section
WAQTC TM 2	Sampling Freshly Mixed Concrete	501
WAQTC FOP for AASHTO T 309	Temperature of Freshly Mixed Hydraulic-Cement Concrete	502
WAQTC FOP for AASHTO T 119	Slump of Hydraulic-Cement Concrete	503
WAQTC FOP for AASHTO T 121	Density (Unit Weight), Yield & Air Content (Gravimetric) of Concrete*	504
WAQTC FOP for AASHTO T 152	Air Content of Freshly Mixed Concrete by the Pressure Method*	505
WAQTC FOP for AASHTO T 23	Making and Curing Concrete Test Specimens in the Field*	506
WAQTC TM 12	Field Sampling and Fabrication of 50–mm (2-in) Cube Specimens using Grout (Non-Shrink) and or Mortar *	507

*This Test Method has an Addendum attached which has specific instructions for the use of the noted test method by the State of Alaska DOT&PF.

Appendix 1 Standard Practice

Title	Description
SP 1	Terminology
SP 2	Calibration of Mechanical Compaction Hammer/ Rammer
SP 3	<i>Reserved for WAQTC Discipline Policy</i>
SP 4	Random Sampling
SP 5	<i>Reserved for Future Use</i>
SP 6	Rounding and Precision in Materials Test Reporting
SP 7	Determination of Outlier Test Results
SP 8	Calibration of Pressure Type Air Meter
SP 9	Deleted
SP 10	Deleted for this publication
SP 11	Contractor Quality Control
SP 12	<i>Reserved for Future Use</i>

Sticks & Roots Content of Aggregate and Soil, ATM 201

1. Scope

This method describes the procedure for determining the percent of sticks & roots by wet mass of the total aggregate or soil sample.

2. Significance

This test would be used to quantify the organic content of soils for particles that are too large to test in accordance with ATM 203, Organic Content of Soils by Ignition.

3. Apparatus

- Balance or scale: Capacity sufficient for the field sample mass, readable to 0.1 percent or 0.1 g and meeting the requirements of AASHTO M 231.
- 2.00 mm (No. 10) sieve conforming to AASHTO M 92.
- Miscellaneous equipment including pans, gloves, etc.

4. Sampling and Sample Preparation

Obtain the sample in accordance with WAQTC FOP for AASHTO T 2. The test will be performed on the complete as-received sample before drying.

5. Procedure

- 5.1. Determine the mass of the as-received sample to 0.1 percent or 0.1 g. Record this as the Total Sample Mass.
- 5.2. Separate the sample on a 2.00 mm (No. 10) sieve to ease identification of sticks & roots.
- 5.3. Separate the sticks & roots from the plus 2.00 mm (No. 10) material and place in a separate pan.
- 5.4. Determine the mass of the sticks & roots to 0.1 percent or 0.1 g. Record this as the Sticks & Roots Mass.

6. Calculations

Calculate the percentage of Sticks & Roots by:
Sticks & Roots, percent =

$$\left(\frac{\text{Sticks \& Roots Wet Mass}}{\text{Total Wet Sample Mass}} \right) \times 100$$

7. Report

Report the Stick and Root Content on Department forms to the nearest 1 percent.

This page left intentionally blank.

**TOTAL EVAPORABLE MOISTURE CONTENT OF AGGREGATE BY DRYING
FOP FOR AASHTO T 255
LABORATORY DETERMINATION OF MOISTURE CONTENT OF SOILS
FOP FOR AASHTO T 265**

Scope

This procedure covers the determination of moisture content of aggregate and soil in accordance with AASHTO T 255 and AASHTO T 265. It may also be used for other construction materials.

Apparatus

- Balance or scale: capacity sufficient for the principle sample mass, accurate to 0.1 percent of sample mass or readable to 0.1 g, and meeting the requirements of AASHTO M 231
- Containers, capable of being sealed
- Suitable drying containers
- Microwave safe containers
- Thermometer reading to $205 \pm 6^{\circ}\text{C}$ ($400 \pm 10^{\circ}\text{F}$)
- Heat source , controlled:
 - Forced draft oven
 - Ventilated / convection oven
- Heat source, uncontrolled:
 - Microwave oven (600 watts minimum)
 - Infrared heater, hot plate, fry pan, or any other device/method that will dry the sample without altering the material being dried
- Utensils such as spoons
- Hot pads or gloves

Sample Preparation

For aggregate, select the proper sample mass, in its existing condition, based on Table 1 or other information that may be specified by the agency. Obtain the sample in accordance with the FOP for AASHTO T 2.

Immediately seal or cover samples to prevent any change in moisture content.

TABLE 1
Sample Sizes for Moisture Content of Aggregate

Nominal Maximum Size* mm (in.)	Minimum Sample Mass g (lb)
4.75 (No. 4)	500 (1.1)
9.5 (3/8)	1,500 (3.3)
12.5 (1/2)	2,000 (4)
19.0 (3/4)	3,000 (7)
25.0 (1)	4,000 (9)
37.5 (1 1/2)	6,000 (13)
50 (2)	8,000 (18)
63 (2 1/2)	10,000 (22)
75 (3)	13,000 (29)
90 (3 1/2)	16,000 (35)
100 (4)	25,000 (55)
150 (6)	50,000 (110)

* One sieve larger than the first sieve to retain more than 10 percent of the material using an agency specified set of sieves based on cumulative percent retained. Where large gaps in specification sieves exist, intermediate sieve(s) may be inserted to determine nominal maximum.

For soil, select the proper sample mass, in its existing condition, based on Table 2 or other information that may be supplied by the agency.

TABLE 2
Sample Sizes for Moisture Content of Soil

Maximum Particle Size mm (in)	Minimum Sample Mass g
0.425 (No. 40)	10
4.75 (No. 4)	100
12.5 (1/2)	300
25.0 (1)	500
50 (2)	1,000

Procedure

For aggregate, determine and record all masses to the nearest 0.1 percent of the sample mass or to the nearest 0.1 g. For soil, determine and record all masses to the nearest 0.1 g. When determining mass, allow the sample and container to cool sufficiently so as not to damage or interfere with the operation of the balance or scale.

1. Determine and record the mass of the container.

2. Place the wet sample in the container and record the total mass of the container and wet sample.
3. Determine the wet mass of the sample by subtracting the mass in Step 1 from the mass in Step 2.
4. Dry the sample to a constant mass in accordance with the directions given under Directions for Drying below. Measures will be taken to protect the scale from excessive heat while determining constant mass.
5. Allow the sample to cool and record the total mass of the container and dry sample.
6. Determine the dry mass of the sample by subtracting the mass in Step 1 from the mass in Step 5.

Directions for Drying Aggregate

- Controlled (forced draft, ventilated or convection oven)

1. Spread sample in the container.
2. Dry to constant mass at $110 \pm 5^{\circ}\text{C}$ ($230 \pm 9^{\circ}\text{F}$). Constant mass has been reached when there is less than a 0.10 percent change after an additional 30 minutes of drying.

- Uncontrolled

Where close control of temperature is not required (such as with aggregate not altered by higher temperatures; with aggregate that will not be used in further tests; or where precise information is not required), higher temperatures or other suitable heat sources may be used. Other heat sources may include microwaves, hot plates, or heat lamps.

— Microwave oven

1. Heap sample in pile in the center of the container and cover. This cover must allow moisture to escape.
2. Dry to constant mass. Constant mass has been reached when there is less than a 0.10 percent change after at least an additional 10 minutes of drying.

Caution: Some minerals in the sample may cause the aggregate to overheat, altering the aggregate gradation.

— Hot plates, heat lamps, etc.

1. Spread sample in container.
2. Stir the sample frequently to avoid localized overheating and aggregate fracturing.
3. Dry to a constant mass. Constant mass has been reached when there is less than a 0.10 percent change after at least an additional 20 minutes of drying.

Directions for Drying Soil

- Oven (preferably forced draft / air)
 1. Place sample in container.
 2. Dry to constant mass at $110 \pm 5^{\circ}\text{C}$ ($230 \pm 9^{\circ}\text{F}$). Constant mass has been reached when there is no change after an additional 1 hour of drying. A sample dried overnight (15 to 16 hours) is sufficient in most cases.

Note 1: Soils containing gypsum or significant amounts of organic material require special drying. For reliable moisture contents dry these soils at 60°C (140°F). For more information see AASHTO T 265, Note 2.

Calculation

Constant Mass for Aggregates:

Calculate constant mass using the following formula:

$$\frac{M_p - M_n}{M_p} \times 100 = \% \text{ Change}$$

Where: M_p = previous mass measurement
 M_n = new mass measurement

Moisture Content Aggregate and Soils:

Calculate the moisture content, as a percent, using the following formula:

$$w = \frac{M_w - M_D}{M_D} \times 100$$

Report

Results shall be reported on standard forms approved for use by the agency. Include:

- M_w , wet mass
- M_D , dry mass
- w , moisture content to nearest 0.1 percent

Addendum WAQTC FOP for AASHTO T 255/ T 265

Following are guidelines for the use of WAQTC FOP for AASHTO T 255/T 265 by the State of Alaska DOT&PF.

1. When drying aggregates, drying overnight shall be sufficient to reach constant mass.

This page intentionally left blank.

Organic Content of Soils ATM 203

1. Scope

This method describes the procedure for determining organic content of soils by loss on ignition as adopted from AASHTO T 267.

This standard involves hazardous materials, operations and equipment. This standard does not purport to address all of the safety problems associated with its use. It is the responsibility of the agency to establish appropriate safety and health practices and to train the user of this standard prior to use. It is the responsibility of the user to consult the appropriate agency authority for and to practice and maintain the appropriate safety and health practices.

2. Apparatus

- 2.00 mm (No. 10) sieve and pan, plus whatever additional larger size sieves are necessary to prevent overloading the No. 10 sieve. Sieves will conform to AASHTO M 92
- Pulverizing apparatus suitable for breaking up aggregations of soil particles without reducing the size of individual grains
- Balance or scale: Capacity sufficient for the principle sample mass, readable to 0.1%, or better, of the total sample mass and meeting the requirements of AASHTO M 231

For this test, this would require a scale with a capacity of at least 100 g and readable to 0.01 g

- Muffle Furnace, thermostatically controlled, capable of maintaining a temperature of $445 \pm 10^{\circ}\text{C}$ ($830 \pm 15^{\circ}\text{F}$). The combustion chamber will be capable of accommodating the designated container(s) and sample(s). The furnace shall be equipped with a pyrometer recorder that will indicate chamber temperature while in use.
- Crucible, with covers, having a minimum volume of 100 ml and capable of withstanding repeated exposure to temperatures of 500°C (950°F)
- Non-asbestos, heat-resistant, gauntlet-type gloves capable of withstanding temperatures of 500°C (950°F)
- Desiccator of sufficient size containing an effective desiccant
- Miscellaneous equipment including tongs, spatulas, wire brushes, etc.

3. Sampling and Sample Preparation

1. Obtain the sample in accordance with WAQTC FOP for AASHTO T 2.
2. Dry the sample to constant mass in accordance with the soil procedure of WAQTC FOP for AASHTO T 255/T 265.
3. Sieve the dry sample through the 2.00 mm (No. 10) sieve.

If the material contains lumps of organics or aggregations of soil, they will be broken up by such means that will not reduce the size of the plus 2.00 mm (No. 10) aggregate particles.

For Topsoil samples: Any large particles of organics that cannot be broken up will be removed and discarded.

Note 1: Organic content for topsoil is the organics that are readily available for use by the root system of the plantings (grass, trees, etc.).

For other types of samples: Any large particles of organics that cannot be broken up will be removed by hand and reported as Sticks and Roots (see ATM 201).

4. Reduce the sample to a mass of approximately 100 g in accordance with WAQTC FOP for AASHTO T 248.

4. Procedure

1. Determine the mass of a crucible to the nearest 0.01 g and record as Tare.
2. Select a sample with a mass between 10-40 g, place into the crucible, determine the mass to the nearest 0.01 g and record as Mass Before Ignition + Tare.

Note 2: Sample masses for lightweight materials such as peat may be less than 10 g but should be of sufficient amount to fill the crucible to at least 3/4 depth. A cover may initially be required over the crucible during the initial phase of ignition to decrease the possibility of the sample being "blown out" from container.

3. Place the crucible into a pre-heated muffle furnace at a temperature of 445°C (835°F) for a minimum of six hours until all organic matter is combusted. If a cover has been used, it shall be removed after approximately 2 hours of combustion.
4. Remove the test sample from the muffle furnace and cool it to room temperature in a desiccator.
5. Determine the mass to the nearest 0.01 grams and record as Mass After Ignition + Tare.

5. Calculations

1. Calculate the percent organic content by the following formula:

$$\text{Organic Content} = \left(\frac{A - B}{A - C} \right) \times 100$$

Where: A = Mass Before Ignition + Tare,
B = Mass After Ignition + Tare,
C = Tare.

6. Report

Report the organic content on Department forms to the nearest 0.1 percent.

DETERMINING THE LIQUID LIMIT OF SOILS WAQTC FOP FOR AASHTO T 89

Scope

This procedure covers the determination of the liquid limit of a soil in accordance with AASHTO T 89. It is used in conjunction with the FOP for AASHTO T 90, Determining the Plastic Limit and Plasticity Index of Soils. The three values are used for soil classification and other purposes.

Apparatus

- Dish: preferably unglazed porcelain or similar mixing dish, about 115 mm (4.5 in.) in diameter.
- Spatula: having a blade 75 to 100 mm (3 to 4 in.) long and about 20 mm (3/4 in.) wide.
- Liquid Limit Device: manually or mechanically operated, consisting of a brass cup, carriage, and base plate.
- Grooving Tool: used to cut the soil in the liquid limit device cup.
- Gauge: part of the grooving tool or a separate metal bar, 10.0 ± 0.2 mm (0.394 ± 0.008 in.) thick and approximately 50 mm (2 in.) long.
- Containers: corrosion resistant, suitable for repeated heating and cooling, having close fitting lids to prevent the loss of moisture. One container is needed for each moisture content determination.
- Balance: conforming to AASHTO M 231, class G1, sensitive to 0.01 g with a 1200 g capacity.
- Oven: thermostatically controlled, capable of maintaining temperatures of $110 \pm 5^\circ\text{C}$ ($230 \pm 9^\circ\text{F}$).
- Graduated cylinders for measuring distilled or demineralized water.

Adjustment of Liquid Limit Device

The liquid limit device shall be inspected to determine that the device is in good working order; that the pin connecting the cup is not worn to permit side play; that the screws connecting the cup to the hanger are tight; that the points of contact on the cup and base are not excessively worn; that the lip of the cup is not excessively worn; and that a groove has not been worn in the cup. The grooving tool shall be inspected to determine that the critical dimensions are correct.

Note 1: Wear is considered excessive when the point of contact on the cup or base exceeds approximately 13 mm (0.5 in.) in diameter, or when any point on the rim of the cup is worn to approximately 1/2 the original thickness. A slight groove in the center of the cup is not objectionable. If the groove becomes pronounced, the cup shall be replaced. A base that is excessively worn may be refinished as long as it is maintained within the tolerances specified.

Adjust the height of drop of the cup so that the point on the cup that comes in contact with the base rises to a height of 10.0 ± 0.2 mm (0.394 ± 0.008 in.).

Note 2: Check the height of the drop, before each new sample, by turning the crank at two revolutions per second while holding the gauge in position against the cup. If a ringing or clicking sound is heard without the cup rising from the gauge, the adjustment is correct. If no ringing is heard or if the cup rises from gauge, readjust the height of the drop. If the cup rocks on the gauge during this checking operation, the cam follower pivot is excessively worn and should be replaced.

Sample

Samples must be prepared per the FOP for AASHTO T 87 or T 146. Obtain a sample with a mass of about 100 g taken from the portion of the material passing the 0.425 mm (No. 40) sieve.

The mass required depends upon the method chosen. Method A (multi-point method) requires approximately 100 g. Method B (single point method) requires approximately 50 g.

Procedure – Method A (Multi-Point)

1. Place the sample in the dish and thoroughly mix with 15 to 20 mL of distilled or demineralized water by alternately and repeatedly stirring, kneading, and chopping with a spatula. Further additions of water shall be in increments of 1 to 3 mL. Each increment shall be thoroughly mixed with the soil before another increment is added. Once testing has begun, no additional dry soil should be added to the moistened soil. The cup of the Liquid Limit device shall not be used for mixing soil and water. If too much water is added, the sample shall either be discarded or mixed and kneaded until natural evaporation lowers the moisture content.

Note 3: Some soils are slow to absorb water. It is possible to add water so fast that a false LL value is obtained. This can be avoided by allowing more mixing and/or time. Also, tap water may be used for routine testing if comparative tests indicate no differences in results between using tap water and distilled or demineralized water.

2. Add sufficient water to form a uniform mass of a stiff consistency.
3. Place enough material in the cup so that, when squeezed and spread with the spatula, the soil will rest in the cup above the spot where the cup rests on the base and will be 10 mm thick at the point of maximum thickness. Use as few strokes of the spatula as possible, taking care to prevent the entrapment of air bubbles in the sample.
4. Divide the soil in the cup with a firm stroke of the grooving tool. Avoid tearing of the sides of the groove or slipping of the soil cake on the cup. Up to six strokes are permitted. The depth of the groove should be increased with each stroke, and only the last stroke should scrape the bottom of the cup.
5. Lift and drop the cup by turning the crank at a rate of approximately two revolutions per second until the two halves of the soil pat come together along a distance of about 13 mm (0.5 in.). Do not hold the base while the crank is turned. Record the number of shocks required to close the groove.

Note 4: Some soils tend to slide on the cup instead of flowing. If this occurs, water should be added, the sample remixed, and the procedure repeated. If the soil continues to slide on the cup, the test is not applicable and a note should be made that the liquid limit could not be determined.

6. Obtain a moisture content sample by slicing through the soil pat perpendicularly with the spatula and through the center of the groove. Place it into a suitable container for subsequent moisture determination.
7. Determine the moisture content of the moisture content sample in accordance with the FOP for AASHTO T 255/T 265 (Soil).
8. Place the soil remaining in the cup back in the mixing dish and add 1 to 3 mL of water, or use previously prepared portions to which sufficient water has been added to result in a more fluid condition.
9. Repeat Steps 3 through 8, a minimum of two times. The object is to have a determination in all three shock ranges 25-35, 20-30, & 15-25.

Flow Curve – Method A

Prepare a flow curve on a semi-logarithmic graph with moisture content on the arithmetic vertical axis and the number of shocks on the logarithmic horizontal axis. The flow curve is a straight line drawn as closely as possible through three or more plotted points.

Liquid Limit – Method A

Determine the liquid limit. The moisture content at the intersection of the flow curve and the 25 shock line is the liquid limit.

Procedure – Method B (Single-Point)

1. Place the sample in the dish and thoroughly mix with 8 to 10 mL of distilled or demineralized water, and following the mixing procedure in Method A, Step 1.
2. Follow the procedure in Method A except that the soil pat should be prepared with water to produce a consistency that will close the two halves of the soil pat at least 13 mm (0.5 in.) within 22 to 28 shocks of the cup.

Note: Groove closures occurring between 15 and 40 blows may be accepted if variations of ± 5 percent of the true liquid limit are tolerable.

3. Return the soil remaining in the cup to the mixing dish and, without adding any additional water, repeat Step 2. If the closure again occurs within the acceptable range, obtain a moisture content specimen.
4. Determine the moisture content of the moisture content sample in accordance with the FOP for AASHTO T 255/T 265 (Soil).

Liquid Limit – Method B

Calculate the liquid limit as follows:

$$LL = (w_N)(N/25)^{0.121}$$

<u>N</u>	<u>(N/25)^{0.121}</u>	<u>N</u>	<u>(N/25)^{0.121}</u>
22	0.985	26	1.005
23	0.990	27	1.009
24	0.995	28	1.014
25	1.000		

$$LL = (w_N)(N/25)^{0.121}$$

where

LL = liquid limit

w_N = moisture content of sample at N blows

N = number of blows

Report

Results shall be reported on standard forms approved by the agency. Report LL to the nearest whole percent.

DETERMINING THE PLASTIC LIMIT AND PLASTICITY INDEX OF SOILS

WAQTC FOP FOR AASHTO T 90

Scope

This procedure covers the determination of the plastic limit and plasticity index of soil in accordance with AASHTO T 90. It is used in conjunction with the FOP for AASHTO T 89, Determining the Liquid Limit of Soils. The three values are used for soil classification and other purposes. This FOP will cover the hand rolling method only. If the plastic limit device method is approved by the agency, see the FOP for AASHTO T 90 for that procedure.

Apparatus

- Dish: preferably unglazed porcelain or similar mixing dish, about 115 mm (4.5 in.) in diameter.
- Spatula: having a blade 75 to 100 mm (3 to 4 in.) long and about 20 mm (3/4 in.) wide.
- Rolling Surface: a ground glass plate or piece of smooth, unglazed paper.
- Containers: corrosion resistant, suitable for repeated heating and cooling, having close fitting lids to prevent the loss of moisture. One container is needed for each moisture content determination.
- Balance: conforming to AASHTO M 231, class G1, sensitive to 0.01 g with a 1200 g capacity.
- Oven: thermostatically controlled, capable of maintaining temperatures of $110 \pm 5^{\circ}\text{C}$ ($230 \pm 9^{\circ}\text{F}$).

Sample

The plastic limit procedure is often run in conjunction with the liquid limit procedure. If this is the case, the plastic limit sample should be obtained from the soil prepared for the liquid limit test at any point in the process at which the soil is plastic enough to be easily shaped into a ball without sticking to the fingers excessively when squeezed. Obtain approximately 8 g of soil to run the plastic limit test.

If the plastic limit only is to be determined, the sample must be prepared per AASHTO T 87 or T 146. Obtain about 20 g of material passing the 0.425 mm (No. 40) sieve. Mix the soil with distilled or demineralized water until the mass becomes plastic enough to be easily shaped into a ball. Obtain approximately 8 g of soil to run the plastic limit test.

Note 1: Tap water may be used for routine testing if comparative tests indicate no differences in results between using tap water and distilled or demineralized water.

Procedure (Hand Rolling Method)

1. From the sample pull a 1.5 to 2 g mass.
2. Squeeze and form the test sample into an ellipsoidal-shape mass.
3. Roll this mass between the fingers or palm and the rolling surface with just sufficient pressure to roll the mass into a thread of uniform diameter along its length. Roll out between 80 and 90 strokes per minute, counting a stroke as one back and forth motion. The sample must be rolled into the 3 mm (1/8 in.) thread in no longer than 2 minutes.

4. Break the thread into six or eight pieces when the diameter of the thread reaches 3 mm (1/8 in.).
5. Squeeze the pieces together between the thumbs and fingers of both hands into an ellipsoidal-shape mass and reroll.
6. Continue this process of alternately rolling to a thread 3 mm (1/8 in.) in diameter, cutting into pieces, gathering together, kneading and rerolling until the thread crumbles under the pressure required for rolling and the soil can no longer be rolled into a thread.

Note 2: Crumbling may occur when the thread has a diameter greater than 3 mm (1/8 in.). This shall be considered a satisfactory end point, provided the soil has been previously rolled into a thread 3 mm (1/8 in.) in diameter. The crumbling will manifest itself differently with various types of soil. Some soils fall apart in many pieces; others form an outside tubular layer that splits at both ends; splitting progresses toward the middle, and the thread falls apart in small platy particles. Heavy clay requires much pressure to deform the thread, particularly as it approaches the plastic limit, and the thread breaks into a series of barrel-shaped segments each 6 to 9 mm (1/4 to 3/8 in.) long. At no time shall the tester attempt to produce failure at exactly 3 mm (1/8 in.) diameter. It is permissible, however, to reduce the total amount of deformation for feebly plastic soils by making the initial diameter of the ellipsoidal-shaped mass nearer to the required 3 mm (1/8 in.) final diameter.

7. Gather the portions of the crumbled soil together and place in a suitable, tared container & cover.
8. Repeat steps one through seven until 8 g of sample have been tested and placed in the covered container.
9. Determine the moisture content of the sample in accordance with the FOP for AASHTO T 255/T 265 (Soil).

Plastic Limit

The moisture content, as determined in Step 9 above, is the Plastic Limit. It is advisable to run several trials on the same material to ensure a proper determination of the Plastic Limit of the soil.

Plasticity Index

The Plasticity Index (PI) of the soil is equal to the difference between the Liquid Limit (LL) and the Plastic Limit (PL).

$$PI = LL - PL$$

Report

Results shall be reported on standard forms approved by the agency. Report the PL and PI to the nearest whole number.

This page intentionally left blank.

pH of Topsoil ATM 206

1. Scope

This method describes the procedure for determining the pH of topsoil.

2. Apparatus

- A soil test kit capable of determining the pH of soils. These are available from commercial greenhouses. Verify reagent expiration dates and replace as needed.
- pH Meter—Calibrate according to manufacturers recommendations.
- 2.00 mm (No. 10) sieve conforming to AASHTO M 92.

3. Sampling and Sample Preparation

- 3.1. Obtain the sample in accordance with WAQTC FOP for AASHTO T 2.
- 3.2. Prepare the soil sample in accordance with the manufacturer's instructions for the soils kit.

4. Procedure

- 4.1. Separate sample on a 2.00 mm (No. 10) sieve. Discard the plus 2.00 mm (No. 10) material unless required for other testing.
- 4.2. Determine the pH of the minus 2.00 mm (No. 10) material in accordance with the manufacturer's instructions.

5. Report

Report the pH value to the nearest 0.5.

This page intentionally left blank.

MOISTURE-DENSITY RELATIONS OF SOILS:

USING A 2.5-kg (5.5-lb) RAMMER AND A 305 mm (12-in.) DROP

FOP FOR AASHTO T 99 (See Addendum for DOT&PF Guidelines)

USING A 4.54-kg (10-lb) RAMMER AND A 457 mm (18-in.) DROP

FOP FOR AASHTO T 180 (See Addendum for DOT&PF Guidelines)

Scope

This procedure covers the determination of the moisture-density relations of soils and soil-aggregate mixtures in accordance with two similar test methods:

- AASHTO T 99: Methods A, B, C, & D
- AASHTO T 180: Methods A, B, C, & D

This test method applies to soil mixtures having 40% or less retained on the 4.75 mm (No 4) sieve for methods A or B, or, 30% or less retained on the 19 mm ($\frac{3}{4}$ "") with methods C or D. The retained material is defined as oversize (coarse) material. If no minimum percentage is specified, greater than 5% will be used. Samples that contain oversize (coarse) material that meet percent retained criteria should be corrected by using the FOP for AASHTO T 224. Samples of soil or soil-aggregate mixture are prepared at several moisture contents and compacted into molds of specified size, using manual or mechanical rammers that deliver a specified quantity of compactive energy. The moist masses of the compacted samples are multiplied by the appropriate factor to determine moist density values. Moisture contents of the compacted samples are determined and used to obtain the dry density values of the same samples. Maximum dry density and optimum moisture content for the soil or soil-aggregate mixture is determined by plotting the relationship between dry density and moisture content.

Apparatus

- Mold – Cylindrical, made of metal and with the dimensions shown in Table 1 or Table 2. It shall include a detachable collar and a base plate to which the mold can be fastened. If permitted by the agency, the mold may be of the “split” type, consisting of two half-round sections, which can be securely locked in place to form a cylinder.
- Rammer –Manually or mechanically-operated rammers as detailed in Table 1 or Table 2. A manually-operated rammer shall be equipped with a guide sleeve to control the path and height of drop. The guide sleeve shall have at least four vent holes no smaller than 9.5 mm ($\frac{3}{8}$ in.) in diameter, spaced approximately 90 degrees apart and approximately 19 mm ($\frac{3}{4}$ in.) from each end. A mechanically-operated rammer will uniformly distribute blows over the sample and will be calibrated with several soil types, and be adjusted, if necessary, to give the same moisture-density results as with the manually operated rammer. For additional information concerning calibration, see the FOP for AASHTO T 99 and T 180.
- Sample extruder – A jack, lever frame, or other device for extruding compacted specimens from the mold quickly and with little disturbance.

- Balance(s) or scale(s) of the capacity and sensitivity required for the procedure used by the agency.

A balance or scale with a capacity of 20 kg (45 lb) and a sensitivity of 5 g (0.01 lb) for obtaining the sample, meeting the requirements of AASHTO M 231.

A balance or scale with a capacity of 2 kg and a sensitivity of 0.1 g is used for moisture content determinations done under both procedures, meeting the requirements of AASHTO M 231.

- Drying apparatus – A thermostatically controlled drying oven, capable of maintaining a temperature of $110 \pm 5^{\circ}\text{C}$ ($230 \pm 9^{\circ}\text{F}$) for drying moisture content samples in accordance with the FOP for AASHTO T 255/T 265.
- Straightedge – A steel straightedge at least 250 mm (10 in.) long, with one beveled edge and at least one surface plane within 0.1 percent of its length, used for final trimming.
- Sieve(s) – 4.75 mm (No. 4) and/or 19.0 mm (3/4 in.), conforming to AASHTO M 92.
- Mixing tools – Miscellaneous tools such as a mixing pan, spoon, trowel, spatula, etc., or a suitable mechanical device, for mixing the sample with water.
- Containers with close-fitting lids to prevent gain or loss of moisture in the sample.

Table 1
Comparison of Apparatus, Sample, and Procedure – Metric

	T 99	T 180
Mold Volume, m ³	Methods A, C: 0.000943	Methods A, C: 0.000943
	Methods B, D: 0.002124	Methods B, D: 0.002124
Mold Diameter, mm	Methods A, C: 101.6	Methods A, C: 101.6
	Methods B, D: 152.4	Methods B, D: 152.4
Mold Height, mm	116.43	116.43
Detachable Collar Height, mm	51	51
Rammer Diameter, mm	50.80	50.80
Rammer Mass, kg	2.495	4.536
Rammer Drop, mm	305	457
Layers	3	5
Blows per Layer	Methods A, C: 25	Methods A, C: 25
	Methods B, D: 56	Methods B, D: 56
Material Size, mm	Methods A, B: 4.75 minus	Methods A, B: 4.75 minus
	Methods C, D: 19.0 minus	Methods C, D: 19.0 minus
Test Sample Size, kg	Method A: 3	Method B: 7
	Method C: 5 ⁽¹⁾	Method D: 11 ⁽¹⁾
Energy, kN-m/m ³	592	2,693

(1) This may not be a large enough sample depending on your nominal maximum size for moisture content samples.

Table 2
Comparison of Apparatus, Sample, and Procedure – English

	T 99	T 180
Mold Volume, ft ³	Methods A, C: 1/30	Methods A, C: 1/30
	Methods B, D: 1/13.33	Methods B, D: 1/13.33
Mold Diameter, in.	Methods A, C: 4.000	Methods A, C: 4.000
	Methods B, D: 6.000	Methods B, D: 6.000
Mold Height, in.	4.584	4.584
Detachable Collar Height, in.	2	2
Rammer Diameter, in.	2.000	2.000
Rammer Mass, lb	5.5	10
Rammer Drop, in.	12	18
Layers	3	5
Blows per Layer	Methods A, C: 25	Methods A, C: 25
	Methods B, D: 56	Methods B, D: 56
Material Size, in.	Methods A, B: No. 4 minus	Methods A, B: No.4 minus
	Methods C, D: 3/4 minus	Methods C, D: 3/4 minus
Test Sample Size, lb	Method A: 7	Method B: 16
	Method C: 12 ₍₁₎	Method D: 25 ₍₁₎
Energy, lb-ft/ft ³	12,375	56,250

(1) This may not be a large enough sample depending on your nominal maximum size for moisture content samples.

Sample

If the sample is damp, dry it until it becomes friable under a trowel. Drying may be in air or by use of a drying apparatus maintained at a temperature not exceeding 60°C (140°F). Thoroughly break up aggregations in a manner that avoids reducing the natural size of individual particles.

Obtain a representative test sample of the mass required by the agency by passing the material through the sieve required by the agency. See Table 1 or Table 2 for test sample mass and material size requirements.

Note 1: Both T 99 & T 180 have four methods (A, B, C, D) that require different masses and employ different sieves.

Note 2: If the sample is plastic (clay types), it should stand for a minimum of 12 hours after the addition of water to allow the moisture to be absorbed. In this case, several samples at different moisture contents should be prepared, put in sealed containers and tested the next day. In instances where the material is prone to degradation, i.e., granular material, a compaction sample with differing moisture contents should be prepared for each point.

Procedure

1. Determine the mass of the clean, dry mold. Include the base plate, but exclude the extension collar. Record the mass to the nearest 0.005 kg (0.01 lb).
2. Thoroughly mix the selected representative sample with sufficient water to dampen it to approximately 4 to 8 percentage points below optimum moisture content. See Note 2.

3. Form a specimen by compacting the prepared soil in the mold (with collar attached) in approximately equal layers. For each layer, spread the loose material uniformly in the mold. Lightly tamp the fluffy material with the manual rammer or other similar device. This establishes a firm surface on which to hold the rammer sleeve. Compact each layer with uniformly distributed blows from the rammer. See Table 1 for mold size, number of layers, number of blows, and rammer specification for the various test methods. Use the method specified by the agency. If material that has not been compacted remains adjacent to the walls of the mold and extends above the compacted surface, trim it down.

Note 3: During compaction, the mold shall rest firmly on a dense, uniform, rigid, and stable foundation or base. This base shall remain stationary during the compaction process.

4. Remove the extension collar. Avoid shearing off the sample below the top of the mold. A rule of thumb is that the material compacted in the mold should not be over 6 mm (¼ in.) above the top of the mold once the collar has been removed.
5. Trim the compacted soil even with the top of the mold with the beveled side of the straightedge.
6. Determine the mass of the mold and wet soil in kg to the nearest 0.005 kg (0.01 lb) or better.
7. Determine the wet mass of the sample by subtracting the mass in Step 1 from the mass in Step 6.
8. Calculate the wet density as indicated below under “Calculations.”
9. Extrude the material from the mold. For soils and soil-aggregate mixtures, slice vertically through the center and take a representative moisture content sample from one of the cut faces, ensuring that all layers are represented. For granular materials, a vertical face will not exist. Take a representative sample. This sample must meet the sample size requirements of the test method used to determine moisture content.

Note 4: When developing a curve for free-draining soils such as uniform sands and gravels, where seepage occurs at the bottom of the mold and base plate, taking a representative moisture content from the mixing bowl may be preferred in order to determine the amount of moisture available for compaction.

10. Determine the moisture content of the sample in accordance with the FOP for AASHTO T 255/T 265.
11. Thoroughly break up the remaining portion of the molded specimen until it will again pass through the sieve, as judged by eye, and add to the remaining portion of the sample being tested. See Note 2.
12. Add sufficient water to increase the moisture content of the remaining soil by approximately 1 to 2 percentage points and repeat steps 3 through 11.
13. Continue determinations until there is either a decrease or no change in the wet density. There will be a minimum of three points on the dry side of the curve and two points on the wet side.

Note 5: In cases of free-draining granular material, the development of points on the wet side of optimum may not be practical.

Calculations

1. Calculate the wet density, in kg/m^3 (lb/ft^3), by multiplying the wet mass from Step 7 by the appropriate factor chosen from the two below.

Methods A & C molds: 1060 (30)

Methods B & D molds: 471 (13.33)

Note 6: The moist mass is in kg (lb). The factors are the inverses of the mold volumes in m^3 (ft^3) shown in Table 1. If the moist mass is in grams, use 1.060 or 0.471 for factors when computing kg/m^3 .

$$1/0.000943 = 1060 \quad [1/(1/30) = 30]$$

$$1/0.002124 = 471 \quad [1/(1/13.33) = 13.33]$$

2. Calculate the dry density as follows.

$$\rho_d = \left(\frac{\rho_w}{w + 100} \right) \times 100 \quad \text{or} \quad \rho_d = \left(\frac{\rho_w}{\frac{w}{100} + 1} \right)$$

Where:

ρ_d = Dry density, kg/m^3 (lb/ft^3)

ρ_w = Wet density, kg/m^3 (lb/ft^3)

w = Moisture content, as a percentage

Moisture-Density Curve Development


32

When dry density is plotted on the vertical axis versus moisture content on the horizontal axis and the points are connected with a smooth line, a moisture-density curve is developed. The coordinates of the peak of the curve are the maximum dry density, or just “maximum density,” and the “optimum moisture content” of the soil.

Example:

Given the following dry density and corresponding moisture content values, develop a moisture-density relations curve and determine maximum dry density and optimum moisture content.

Dry Density		Moisture Content, %
kg/m ³	lb/ft ³	
1846	114.3	11.3
1868	115.7	12.1
1887	116.9	12.8
1884	116.7	13.6
1871	115.9	14.2

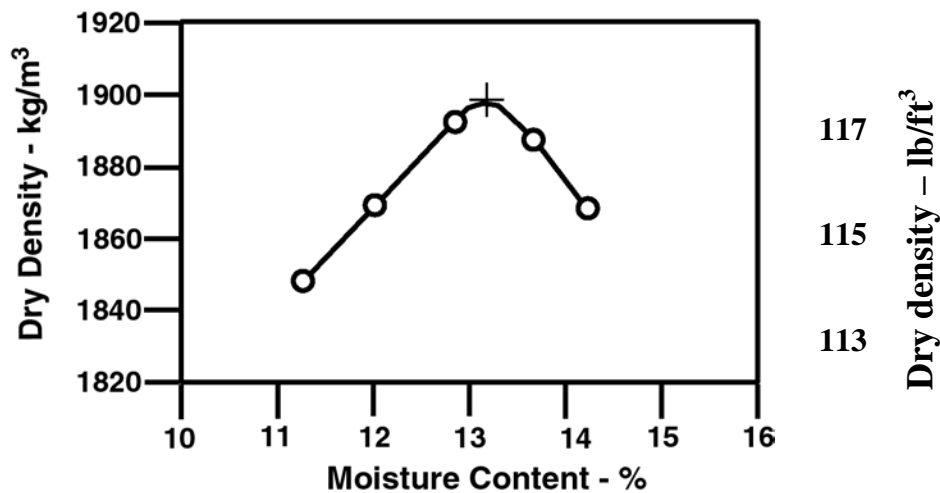

In this case, the curve has its peak at:

Maximum dry density = 1890 kg/m³ (117.0 lb/ft³)

Optimum water content = 13.2%

Note that both values are approximate, since they are based on sketching the curve to fit the points.

Report

Results shall be reported on standard forms approved by the agency. Report maximum dry density to the closest 1 kg/m³ (0.1 lb/ft³) and optimum moisture content to the closest 0.1 percent.

Addendum WAQTC FOP for AASHTO T 99/ T 180

Following are guidelines for the use of WAQTC FOP for AASHTO T 99/T 180 by the State of Alaska DOT&PF.

1. Moisture content shall be determined using the mass requirements listed in table 2 of WAQTC FOP for AASHTO T 255/T 265.
2. In order to properly draw the moisture-density curve, it may be helpful to plot a Zero Air Voids (ZAV) curve. The ZAV curve must be to the right of the wet side of the curve. To plot the curve, you will need to establish the specific gravity of the soil. Specific gravity of the soil can be estimated, assumed to be 2.700, or it can be determined in accordance with AASHTO T 100.
3. The points for plotting the ZAV shall be calculated by selecting dry unit masses and calculating a corresponding moisture content value as follows:

$$W_s = \frac{(\gamma_w)G_s - \gamma_d}{(\gamma_d)(G_s)} \times 100$$

Where:

W_s = Water content for complete saturation, %

γ_w = Unit Mass of water 9.789 kN/m³ (62.4 lbf/ft³)

γ_d = Dry unit mass of soil, kN/m³ (lbf/ft³)

G_s = Specific Gravity of soil or G_{avg} from Addendum item 4.

4. When the material includes plus 4.75 mm (No. 4) materials, the plus 4.75 mm (No. 4) specific gravity may be estimated, assumed to be 2.700 or it can be tested in accordance with WAQTC FOP for AASHTO T 85. If a weighted average is used, it shall be calculated as follows:

$$G_{avg} = \frac{1}{\frac{R_1}{100G_1} + \frac{P_1}{100G_2}}$$

Where:

G_{avg} = Weighted average specific gravity of soils

R_1 = Percent of soil particles retained on the 4.75 mm (No. 4) sieve

P_1 = Percent of soil particles passing the 4.75 mm (No. 4) sieve

G_1 = Apparent specific gravity of soil particles retained on the 4.75 mm (No. 4) sieve

G_2 = Specific gravity of soil particles passing the 4.75 mm (No. 4) sieve

5. Unless stated otherwise, T 180 shall be used.
6. The use of an extruder is optional when the sample being tested is granular.

This page intentionally left blank.

Determining the Standard Density of Coarse Granular Materials Using the Vibratory Compactor ATM 212

1. Scope

This method determines the maximum density values of granular materials for a standard compaction energy. The method accounts for variations in the maximum attainable density of a given material due to fluctuations in gradation.

With the specific gravity and the compacted density of the plus 4.75 mm (no. 4) and the minus 4.75 mm (No. 4) fractions, a chart and/or curve of standard density values versus percent passing the No. 4 sieve can be plotted.

This test method is conducted using the minus 75 mm (3 in) portion of the sample. It applies to soils having 10-80 percent passing the 4.75 mm (No. 4) sieve and with the minus 4.75 mm (No. 4) portion of the sample having 10 percent or less passing the 75 μ m (No. 200) sieve.

Note 1: The Vibratory Compaction Test was developed for sandy gravels whose fine fraction is non-plastic and highly permeable or free draining. When the fine fraction is primarily a soil with some plasticity and low permeability or not free draining, WAQTC FOP for AASHTO T 99/T 180 will be used. With borderline materials, both tests shall be applied, and the one yielding the highest unit weight value will be used.

2. Apparatus

- A vibratory spring-loaded compactor essentially conforming to specifications that can be obtained from the State Materials Engineer.
- Standard Mold and base with and a piston to fit inside the mold with a maximum 1.5 mm (1/16 in) clearance between piston and mold.
- A 0.014 m³ (1/2 ft³) mold with a piston to fit inside mold having a maximum 1.5 mm (1/16 in) clearance between piston and mold.

Note 2: The molds and pistons will be constructed of metal of such dimensions as to remain rigid and inflexible under test conditions.

- Spacer blocks of varying heights compatible with the compactor and pistons.
- Measuring device, accurate and readable to 0.1 mm (0.01 in) with a minimum 300 mm (6 in) length.
- A 75 mm (3 in) and a 4.75 mm (No. 4) sieve conforming to AASHTO M 92 requirements.
- Balance or scale: Capacity sufficient for the principle sample mass, readable to 0.1 percent or 0.1 g and meeting the requirements of AASHTO M 231.

Note 3: For the fine aggregate compaction test, this would require a scale with a capacity of at least 20 kg (45 lb) and readable to 5 g (0.01 lb) or better.

Note 4: For the fine aggregate moisture content, this would require a scale with a capacity of at least 1000 g and readable to 0.1 g or better.

Note 5: For the coarse aggregate compaction test, this would require a scale with a capacity of at least 20 kg (45 lb) and readable to 5 g (0.01 lb) or better.

- A 2.5 kg (5.5 lb) metal rammer conforming to the requirements of WAQTC FOP for AASHTO T 99/T 180.

- Tamping rod of straight steel, 16 mm (5/8 in) in diameter and approximately 400 mm (24 in) long having at least one end rounded to a hemispherical tip.
- Graduated cylinder, 1000 ml capacity, readable to 5 ml.
- A stopwatch or timer accurate to 1 second.
- Miscellaneous tools including pans, spoon, trowel, mechanical mixer (optional), etc.

3. Equipment Calibration

Calibration data will be updated annually or more frequently if justified by use. Calibration information will be recorded and accessible for every test.

Calibration of the Standard Mold:

1. Measure the top and bottom diameter of the mold to the nearest 0.1 mm (0.01 in) and average the results to obtain the mean diameter of the mold. Calculate the area of the average diameter by the formula:

$$A = \pi \times (0.5 \times d)^2$$

Where:

A = Area of mean diameter, in² or mm²,

π = 3.1416,

d = mean diameter, in or mm.

2. Assemble the mold, measure the overall height of the mold to the nearest 0.1 mm (0.01 in) at least 4 different places around the circumference of the mold and average the measurements. Record this as Height of Mold.
3. Calculate the Mold Conversion Factor by:

$$C = \frac{1,000,000,000}{A} \text{ or } \frac{1728}{A} \text{ USC}$$

Where:

C = Mold Conversion Factor, (1,000,000,000 = mm³/m³ and 1728 = in³/ft³),

A = Area of mean diameter.

4. Record the result as the Small Mold Conversion Factor to 0.01.
5. Calibration of the 0.014 m³ Mold (Large): Calibrate this mold using the same procedure as described for the small mold above and record the result to 0.01 as the Large Mold Conversion Factor.

4. Sample Preparation

1. Sample the material in accordance with WAQTC FOP for AASHTO T 2. Prepare the field sample by splitting out a representative portion in accordance with WAQTC FOP for AASHTO T 248, Method A, to provide sufficient material for the following tests.
 - Sieve Analysis in accordance with WAQTC FOP for AASHTO T 27/T 11.
 - Coarse Aggregate Apparent Specific Gravity in accordance with WAQTC FOP for AASHTO T 85.
 - Fine Aggregate Apparent Specific Gravity in accordance with AASHTO T 84 or AASHTO T100.
 - Compaction sample to provide sufficient material for the compaction specimens detailed below.
2. Dry the compaction sample to constant mass in accordance with WAQTC FOP for AASHTO T 255.

3. Scalp the plus 75 mm (3 in) material from the compaction sample and discard, if not needed for any other tests. Separate the remainder of the compaction sample into coarse [minus 75 mm (3 in) to 4.75 mm (No. 4)] and fine [minus 4.75 mm (No. 4)] aggregate portions.
4. The quantity of material necessary to complete tests on both fractions is:
 - a. Fine aggregate, minimum of 3 portions approximately 6 kg (13 lb) each.
 - b. Coarse aggregate:
 - 1) For material containing 5 percent or less of 19.0 mm (3/4 in) material, a portion of the minus 19.0 mm (3/4 in) aggregate of approximately 6 kg (13 lb).
 - 2) For material containing more than 5 percent plus 19.0 mm (3/4 in) aggregate a portion of 18 to 20 kg (40 to 45 lb).

5. Procedure

1. Compaction Test of the Fine Fraction
 - a. Assemble the Standard Mold and determine its mass, along with the Piston, to the nearest 5 g (0.01 lb). Record this as the Mass of Mold Assembly.
 - b. Using one of the fine aggregate portions, add an amount of water estimated to produce a saturated sample when compacted and mix thoroughly.
 - 1) When the material is at its saturation point, free water (a drop or two) will show at the base of the mold at about the 227 kg (500 lb) load of the first compression run. The ideal saturation point would be a bead of water around the base of the mold at the end of the 10-minute compaction run. Most materials will yield the highest density at that moisture content. Some materials may continue to gain density at higher moisture contents; however, this is due to the washing out of fines, which will alter the character of the sample. Therefore, if severe washing-out or pumping of fines occurs (as evidenced by dirty water flooding off of the base or pumped on top of the piston), the sample is beyond the saturation point, will be discarded and a lower moisture content tried for the saturation point.
 - 2) Moisture contents beyond the saturation point need not be tested.
 - c. Set the piston aside and place the sample in the mold in three approximately equal layers. Consolidate each lift by 25 strokes of the tamping rod followed by 25 blows of the manual rammer. If severe displacement of the material occurs, adjust the blow strength by limiting the height of each blow to produce the maximum compaction and minimum displacement. The surface of the top lift should be finished as level as possible.
 - d. Place the piston on top of the sample and mount the mold on the jack platform in the compactor. Spacers between the load spring and piston must be used to adjust the elevation of the mold so the hammers strike the mold in the center of the lift area. Elevate the mold until the loading head seats on top of the piston. Apply an initial seating load of approximately 45 kg (100 lbs) on the sample.
 - e. Start the vibratory hammers and, by elevating the jack, begin the loading rate procedure.

The load application rate to 2000 lbs. is applied as follows:

Load	Elapsed Time
0 to 225 kg (500 lb)	1 minute
225 kg to 450 kg (1000 lb)	1-1/2 minutes
450 kg to 900 kg (2000 lb)	2 minutes

- f. Upon reaching the 900 kg (2000 lb) load at the end of the 2-minute cycle, stop the hammers, release the load on the jack, and return to zero pressure.
 - g. Repeat Steps (e) and (f) four additional times. After the last run remove the mold from the compactor.
 - h. Measure the height of the compacted sample, to the top of the piston, to the nearest 0.1 mm (0.01 in) by measuring from the top of the mold to the surface of the sample at a minimum of 4 different places evenly spaced around the circumference of the mold. Record and average these measurements. Subtract this average from the overall height of the mold and record as the Height of Sample.
 - i. Determine the mass of the specimen in the mold to the nearest 5 g (0.01 lb). Record this as Mass of Mold Assembly + Aggregate.
 - j. Remove the specimen from the mold and determine the moisture content in accordance with WAQTC FOP for AASHTO T 255, recording the data on the Vibratory Compaction Worksheet.
 - k. Repeat Steps (b) thru (j) at lower or higher moisture content increments of approximately 1 percent intervals to determine the maximum density value for the material. Three tests are usually sufficient.
2. Compaction Test of the Coarse Fraction:
- a. For minus 19 mm (3/4 in) aggregates:
 - 1) Determine the mass of the coarse aggregate to the nearest 5 g (0.01 lb). Record this mass as Net Mass of Coarse Aggregate.
 - 2) Add 2.5 percent moisture to the sample, mix thoroughly and place in the Standard CBR mold in approximately three equal lifts. Compact each lift with 25 blows of the tamping rod (omit hammering). Avoid the loss of any material during this operation, or the net mass of coarse aggregate must be determined again, after determining the height of the sample and drying the material to constant mass.
 - 3) Follow the procedures outlined in steps 1d. through 1h.
 - b. For plus 19 mm (3/4 in) aggregates:
 - 1) Determine the mass of the coarse aggregate to the nearest 5 g (0.01 lb) or better. Record this mass the Net Mass of Coarse Aggregate.
 - 2) Divide the sample into three representative and approximately equal portions.
 - 3) Place one of the portions into the 0.014 m³ (1/2 ft³) mold. Level the surface by hand and consolidate the layer with 25 strokes of the tamping rod, using the rounded end. Distribute the strokes evenly over the entire cross section of the material rodding full depth, if possible, without hitting the bottom too hard.

- 4) Repeat this procedure for the other lifts, penetrating, if possible, into the lower layer. Avoid the loss of any material during this operation, or the net mass of coarse aggregate must be re-determined after determining the height of the sample. Position the piston on the sample, mount the mold in the compactor and follow the procedure described in steps 1d. through 1h.

6. Calculations

1. Determine the dry density of each of the fine aggregate points as follows:

- a. Calculate the net mass of aggregate by:

$$e = c - d$$

Where:

- e = net mass of aggregate, kg (lb)
- c = mass of mold assembly + aggregate, kg (lb)
- d = mass of mold assembly.

- b. Calculate the wet density by:

$$g = \frac{e \times b}{f}$$

Where:

- g = wet unit weight, kg/m³ (lb/ft³)
- e = net mass of aggregate, kg (lb)
- b = mold conversion factor, metric (USC), and
- f = height of sample, mm (in).

- c. Calculate the dry density of each of the fine fraction specimens as follows:

$$h = \frac{g}{1 + n}$$

Where:

- h = dry density for moisture content n, kg/m³ (lb/ft³)
- g = wet density, kg/m³ (lb/ft³)
- n = moisture content, expressed as a decimal.

- d. The maximum dry density (D_f) for the fine fraction is the highest density at or below the saturation point.

2. Calculate the maximum dry density (D_c) of the coarse fraction by:

$$D_c = \frac{u \times r}{v}$$

Where:

- D_c = dry unit weight, kg/m³ (lb/ft³)
- u = net mass of aggregate, kg (lb)
- r = mold conversion factor, metric (USC)
- v = height of sample, mm (in).

3. Determine the apparent specific gravity of the fine aggregate in accordance with AASHTO T 84.
4. Determine the apparent specific gravity of the coarse aggregate in accordance with WAQTC FOP for AASHTO T 85.

5. Plotting the "Maximum Dry Density vs. the Percent Passing 4.75 mm (No. 4) Sieve" curve is based on complex theoretical formulae. Programs for solution of these formulae, which produce curve data points and charts, have been developed for spreadsheets. These programs are available from the Statewide/ Regional laboratories.

7. Report

The results shall be reported on Department forms. In addition to the standard conformance tests for the material, the Maximum Dry Density shall be reported in chart form to the nearest 1 kg/m^3 (0.1 lb/ft^3) vs. the Percent Passing 4.75 mm (No. 4) in whole percentages from 0 to 100 percent. The data may be displayed graphically in addition to the chart.

IN-PLACE DENSITY AND MOISTURE CONTENT OF SOIL AND SOIL-AGGREGATE BY NUCLEAR METHODS (SHALLOW DEPTH) (See Addendum for DOT&PF Guidelines) **FOP FOR AASHTO T 310**

Scope

This procedure covers the determination of density, moisture content, and relative compaction of soil, aggregate, and soil-aggregate mixes in accordance with AASHTO T 310. This field operating procedure is derived from AASHTO T 310. The nuclear moisture-density gauge is used in the direct transmission mode.

Apparatus

- Nuclear density gauge with the factory matched standard reference block.
- Drive pin, guide/scrapper plate, and hammer for testing in direct transmission mode.
- Transport case for properly shipping and housing the gauge and tools.
- Instruction manual for the specific make and model of gauge.
- Radioactive materials information and calibration packet containing:
 - Daily Standard Count Log.
 - Factory and Laboratory Calibration Data Sheet.
 - Leak Test Certificate.
 - Shippers Declaration for Dangerous Goods.
 - Procedure Memo for Storing, Transporting and Handling Nuclear Testing Equipment.
 - Other radioactive materials documentation as required by local regulatory requirements.
- Sealable containers and utensils for moisture content determinations.

Radiation Safety

This method does not purport to address all of the safety problems associated with its use. This test method involves potentially hazardous materials. The gauge utilizes radioactive materials that may be hazardous to the health of the user unless proper precautions are taken. Users of this gauge must become familiar with the applicable safety procedures and governmental regulations. All operators will be trained in radiation safety prior to operating nuclear density gauges. Some agencies require the use of personal monitoring devices such as a thermoluminescent dosimeter or film badge. Effective instructions together with routine safety procedures such as source leak tests, recording and evaluation of personal monitoring device data, etc., are a recommended part of the operation and storage of this gauge.

Calibration

Calibrate the nuclear gauge as required by the agency. This calibration may be performed by the agency using manufacturer's recommended procedures or by other facilities approved by the agency. Verify or re-establish calibration curves, tables, or equivalent coefficients every 12 months.

Standardization

1. Turn the gauge on and allow it to stabilize (approximately 10 to 20 minutes) prior to standardization. Leave the power on during the day's testing.
2. Standardize the nuclear gauge at the construction site at the start of each day's work and as often as deemed necessary by the operator or agency. Daily variations in standard count shall not exceed the daily variations established by the manufacturer of the gauge. If the daily variations are exceeded after repeating the standardization procedure, the gauge should be repaired and or recalibrated.
3. Record the standard count for both density and moisture in the Daily Standard Count Log. The exact procedure for standard count is listed in the manufacturer's Operators Manual.

Note 1: New standard counts may be necessary more than once a day. See agency requirements.

Overview

There are two methods for determining in-place density of soil / soil aggregate mixtures. See agency requirements for method selection.

- Method A Single Direction
- Method B Two Direction

Procedure

1. Select a test location(s) randomly and in accordance with agency requirements. Test sites should be relatively smooth and flat and meet the following conditions:
 - a. At least 10 m (30 ft) away from other sources of radioactivity
 - b. At least 3 m (10 ft) away from large objects
 - c. The test site should be at least 150 mm (6 in.) away from any vertical projection, unless the gauge is corrected for trench wall effect.
2. Remove all loose and disturbed material, and remove additional material as necessary to expose the top of the material to be tested.
3. Prepare a flat area sufficient in size to accommodate the gauge. Plane the area to a smooth condition so as to obtain maximum contact between gauge and the material being tested. For Method B, the flat area must be sufficient to permit rotating the gauge 90 or 180 degrees about the source rod.
4. Fill in surface voids beneath the gauge with native fines passing the 4.75 mm (No. 4) sieve or finer. Smooth the surface with the guide plate or other suitable tool. The depth of the native fines filler should not exceed approximately 3 mm (1/8 in.).
5. Make a hole perpendicular to the prepared surface using the guide plate and drive pin. The hole shall be at least 50 mm (2 in.) deeper than the desired probe depth, and shall be aligned such that

insertion of the probe will not cause the gauge to tilt from the plane of the prepared area. Remove the drive pin by pulling straight up and twisting the extraction tool.

6. Place the gauge on the prepared surface so the source rod can enter the hole without disturbing loose material.
7. Insert the probe in the hole and lower the source rod to the desired test depth using the handle and trigger mechanism.
8. Seat the gauge firmly by partially rotating it back and forth about the source rod. Ensure the gauge is seated flush against the surface by pressing down on the gauge corners, and making sure that the gauge does not rock.
9. Pull gently on the gauge to bring the side of the source rod nearest to the scaler/detector firmly against the side of the hole.
10. Perform one of the following per agency requirements:
 - a. **Method A Single Direction:** Take a test consisting of the average of two, one minute readings, and record both density and moisture data. The two wet density readings should be within 32 kg/m^3 (2.0 lb/ft^3) of each other. The average of the two wet densities and moisture contents will be used to compute dry density.
 - b. **Method B Two Direction:** Take a one-minute reading and record both density and moisture data. Rotate the gauge 90 degrees or 180, pivoting it around the source rod. Reseat the gauge by pulling gently on the gauge to bring the side of the source rod nearest to the scaler/detector firmly against the side of the hole and take one-minute reading. (In trench locations, rotate the gauge 180 degrees for the second test.) Some agencies require multiple one-minute readings in both directions. Analyze the density and moisture data. A valid test consists of wet density readings in both gauge positions that are within 50 kg/m^3 (3.0 lb/ft^3). If the tests do not agree within this limit, move to a new location. The average of the wet density and moisture contents will be used to compute dry density.
11. If required by the agency, obtain a representative sample of the material, 4 kg (9 lb) minimum, from directly beneath the gauge full depth of material tested. This sample will be used to verify moisture content and / or identify the correct density standard. Immediately seal the material to prevent loss of moisture.

The material tested by direct transmission can be approximated by a cylinder of soil approximately 300 mm (12 in.) in diameter directly beneath the centerline of the radioactive source and detector. The height of the cylinder will be approximately the depth of measurement. When organic material or large aggregate is removed during this operation, disregard the test information and move to a new test site.
12. To verify the moisture content from the nuclear gauge, determine the moisture content with a representative portion of the material using the FOP for AASHTO T 255/T 265 . If the moisture content from the nuclear gauge is within $\pm 1\%$, the nuclear gauge readings can be accepted. Retain the remainder of the sample at its original moisture content for a one-point compaction test under the FOP for AASHTO T 272, or for gradation, if required.

Note 2: Example: A Gauge reading of 16.8% moisture and an oven dry of 17.7% are within the $\pm 1\%$ requirements. Moisture correlation curves will be developed according to agency guidelines. These curves should be reviewed and possibly redeveloped every 90 days.
13. Determine the dry density by one of the following.

- a. From nuclear gauge readings, compute by subtracting the mass (weight) of the water (kg/m^3 or lb/ft^3) from the wet density (kg/m^3 or lb/ft^3) or compute using the % moisture by dividing wet density from the nuclear gauge by $1 + \text{moisture content expressed as a decimal}$.
- b. When verification is required and the nuclear gauge readings cannot be accepted, the moisture content is determined by the FOP for AASHTO T 255/T 265, compute dry density by dividing wet density from the nuclear gauge by $1 + \text{moisture content expressed as a decimal}$.

Percent Compaction

- Percent compaction is determined by comparing the in-place dry density as determined by this procedure to the appropriate agency density standard. For soil or soil-aggregate mixes, these are moisture-density curves developed using the FOP for AASHTO T 99/ T 180. When using curves developed by the FOP for AASHTO T 99 / T 180, it may be necessary to use the FOP for AASHTO T 224 and FOP for AASHTO T 272 to determine maximum density and moisture determinations.

For coarse granular materials, the density standard may be density-gradation curves developed using a vibratory method such as AKDOT&PFs ATM 212, ITD's T 74, WSDOT's TM 606, or WFLHDs Humphrys.

See appropriate agency policies for use of density standards.

Calculate the dry density as follows:

$$\rho_d = \left(\frac{\rho_w}{w + 100} \right) \times 100 \quad \text{or} \quad \rho_d = \left(\frac{\rho_w}{\frac{w}{100} + 1} \right)$$

Where:

ρ_d = Dry density, kg/m³ (lb/ft³)

ρ_w = Wet density, kg/m³ (lb/ft³)

w = Moisture content from the FOP for AASHTO T 255 / T 265 as a percentage

Report

Results shall be reported on standard forms approved by the agency. Include the following information:

- Location of test, elevation of surface, and thickness of layer tested.
- Visual description of material tested.
- Make, model and serial number of the nuclear moisture-density gauge.
- Wet density to 0.1 lb/ft³.
- Moisture content as a percent, by mass, of dry soil mass to 0.1 percent.
- Dry density to 0.1 lb/ft³.
- Standard density to 0.1 lb/ft³.
- Percent compaction.
- Name and signature of operator.

Addendum WAQTC for AASHTO T 310

Following are guidelines for the use of WAQTC FOP for AASHTO T 310 by the State of Alaska DOT&PF.

1. The procedure designated as Method A will be used.
2. Calculate the percent compaction as follows:

$$\%D_{\max} = \left(\frac{\rho_d}{\rho_{\max}} \right) \times 100$$

Where:

$\%D_{\max}$ = Percent Compaction

ρ_d = Dry Density, kg/m³ (lb/ft³)

ρ_{\max} = Standard Density or Corrected Standard Density if WAQTC FOP for AASHTO T 224 is used.

3. Report percent compaction to the nearest whole percent.
4. The visual description of the material will be the material classification, i.e. Borrow, D-1, etc.
5. The offset factor (k) shall be used to correct the moisture content reading from the gauge.
 - a. Determine the offset factor (k) by:
 - 1) Average minimum five gauge derived moisture contents. .
 - 2) Average minimum five moisture contents determined by WAQTC FOP for AASHTO T 255/T 265 taken from the locations used to determine the gauge derived moistures.
 - 3) Calculate the offset factor (k) using the following formula.

$$k = \frac{\%M_{LAB} - \%M_{GAUGE}}{100 + \%M_{GAUGE}} \times 1000$$

- b. Follow the gauge Manufacturer's instructions to enable the offset function to correct the moisture reading.
- c. Be sure to disengage the offset function upon completion of test.

Note: This procedure is set up for Troxler gauges.

6. A representative sample of material is required from beneath the gauge for purposes of: verification of moisture content for nuclear gauge according to WAQTC FOP for T 310; correcting the Standard Density determined by WAQTC FOP for T 99/T 180, according to WAQTC FOP for T 224 when greater than 5% coarse particles are present; and determining the minus No. 4 for ATM 212.

A sample of material will not be required when any one of the following conditions applies:

- a. The Standard Density is determined by ATM 212, and the test meets the minimum density requirement using the maximum density from the peak of the curve.
- b. The Project Engineer may waive this requirement when testing top layer of surface course and the Standard Density is determined using WAQTC FOP for AASHTO T 99/T 180. In this case, the

percent coarse (oversized) for calculating the corrected density shall be established from prior gradations representing the material being tested.

- c. A sample is not required for moisture content when the nuclear gauge moisture has been determined to be within 1% of the oven dry moisture and is verified at the required frequency.

This page intentionally left blank

CORRECTION FOR COARSE PARTICLES IN THE SOIL COMPACTION TEST

WAQTC FOP FOR AASHTO T 224 (See Addendum for DOT&PF Guidelines)

Scope

This procedure covers the adjustment of the maximum dry density determined by FOP for AASHTO T 99 / T 180 to compensate for coarse particles retained on the 4.75 mm (No. 4) or 19.0 mm (3/4 in.) sieve. For Methods A and B of the FOP for AASHTO T 99 / T 180 the adjustment is based on the percent, by mass, of material retained on the 4.75 mm (No. 4) sieve and the bulk specific gravity (G_{sb}) of the material retained on the 4.75 mm (No. 4) sieve. A maximum of 40% of the material can be retained on the 4.75 mm (No. 4) sieve for this method to be used. For Methods C and D of the FOP for AASHTO T 99 / T 180, the adjustment is based on the percent, by mass, of material retained on the 19.0 mm (3/4 in.) sieve and the bulk specific gravity (G_{sb}) of the material retained on the 19.0 mm (3/4 in.) sieve. A maximum of 30% of the material can be retained on the 19.0 mm (3/4 in.) sieve for this method to be used. Whether the split is on the 4.75 mm (No. 4) or the 19.0 mm (3/4 in.) sieve, all material retained on that sieve is defined as oversized material.

This method applies to soils with percentages up to the maximums listed above for oversize particles. A correction may not be practical for soils with only a small percentage of oversize material. The agency shall specify a minimum percentage below which the method is not needed. If not specified, this method applies when more than 5 percent by weight of oversize particles is present.

Adjustment Equation

Along with density, the moisture content can be corrected. The moisture content can be determined by the FOP for AASHTO T 255 / T 265, other agency approved methods, or the nuclear density gauge moisture content reading from the FOP for AASHTO T 310. If the nuclear gauge moisture reading is used, or when the moisture content is determined on the entire sample (both fine and oversized particles), the use of the adjustment equation is not needed. Combined moisture contents with material having an appreciable amount of silt or clay should be performed using FOP for AASHTO T 255 / T 265 (Soil). Moisture contents used from FOP for AASHTO T 310 must meet the criteria for that method.

When samples are split for moisture content (oversized and fine materials) the following adjustment equations must be followed:

1. Split the sample into oversized material and fine material.
2. Dry the oversized material following the FOP for AASHTO T 255 / T 265 (Aggregate). If the fine material is sandy in nature, dry using the FOP for AASHTO T 255 / T 265 (Aggregate), or other agency approved methods. If the fine material has any appreciable amount of clay, dry using the FOP for AASHTO T 255 / T 265 (Soil) or other agency approved methods.
3. Calculate the dry mass of the oversize and fine material as follows:

$$M_D = \frac{M_m}{(1 + MC)}$$

Where:

M_D = mass of dry material (fine or oversize particles).

M_m = mass of moist material (fine or oversize particles).

MC = moisture content of respective fine or oversized, expressed as a decimal.

4. Calculate the percentage of the fine and oversized particles by dry weight of the total sample as follows: See Note 2.

$$P_f = \frac{100 M_{DF}}{(M_{DF} + M_{DC})}$$

And

$$P_c = \frac{100 M_{DC}}{(M_{DF} + M_{DC})}$$

Or for P_c : $P_c = 100 - P_f$

Where:

P_f = percent of fine particles, of sieve used, by weight.

P_c = percent of oversize particles, of sieve used, by weight.

M_{DF} = mass of fine particles.

M_{DC} = mass of oversize particles.

5. Calculate the corrected moisture content as follows:

$$MC_T = \frac{[(MC_F)(P_f) + (MC_c)(P_c)]}{100}$$

MC_T = corrected moisture content of combined fines and oversized particles, expressed as a % moisture.

MC_F = moisture content of fine particles, as a % moisture.

MC_c = moisture content of oversized particles, as a % moisture.

Note 1: Moisture content of oversize material can be assumed to be two (2) percent for most construction applications.

Note 2: In some field applications agencies will allow the percentages of oversize and fine materials to be determined with the materials in the wet state.

Adjustment Equation Density

6. Calculate the corrected dry density of the total sample (combined fine and oversized particles) as follows:

$$D_d = \frac{100 D_f k}{[(D_f)(P_c) + (k)(P_f)]} \quad \text{or} \quad D_d = \frac{100}{\frac{P_f}{D_f} + \frac{P_c}{k}}$$

Where:

D_d = corrected total dry density (combined fine and oversized particles) kg/m^3 (lb/ft^3).

D_f = dry density of the fine particles kg/m^3 (lb/ft^3), determined in the lab.

P_c = percent of oversize particles, of sieve used, by weight.

P_f = percent of fine particles, of sieve used, by weight.

k = Metric:

1,000 * Bulk Specific Gravity (G_{sb})
(oven dry basis) of coarse particles (kg/m^3).

k = English:

62.4 * Bulk Specific Gravity (G_{sb})
(oven dry basis) of coarse particles (lb/ft^3).

Note 3: If the specific gravity is known, then this value will be used in the calculation. For most construction activities the specific gravity for aggregate may be assumed to be 2.600.

Report

Results shall be reported on standard forms approved by the agency. Report adjusted maximum dry density to the closest 1 kg/m^3 (0.1 lb/ft^3).

Addendum WAQTC FOP for AASHTO T 224

Following are guidelines for the use of WAQTC FOP for AASHTO T 224 by the State of Alaska DOT&PF.

1. The maximum allowable oversized (+19 mm (3/4 in)) material is 40 percent. The maximum dry density to be used with material containing 30 to 40 percent oversized is the oversized correction calculated at 30 percent.
2. When testable materials have more than 40% retained on the 19mm (3/4 in) sieve, record the percent oversize, the moisture content, and record the test as Too Coarse To Test (TCTT).
3. When results are used for acceptance, the Specific Gravity shall be determined.

SAMPLING OF AGGREGATES (See Addendum for DOT&PF Guidelines) **FOP FOR AASHTO T 2**

Scope

This procedure covers sampling of coarse, fine, or a combination of coarse and fine aggregates (CA and FA) in accordance with AASHTO T 2. Sampling from conveyor belts, transport units, roadways, and stockpiles is covered.

Apparatus

- Shovels and/or scoops
- Sampling tubes of acceptable dimensions
- Mechanical sampling systems: normally a permanently attached device that allows a sample container to pass perpendicularly through the entire stream of material or diverts the entire stream of material into the container by manual, hydraulic, or pneumatic operation
- Belt template
- Sampling containers

Procedure - General

Sampling is as important as testing, and the technician shall use every precaution to obtain samples that will show the true nature and condition of the materials the sample represents. In all situations, determine the time or location for sampling in a random manner.

1. Wherever samples are taken, obtain multiple increments of approximately equal size.
2. Mix the increments thoroughly to form a field sample that meets or exceeds the minimum mass recommended in Table 1.

TABLE 1
Sample Sizes

Nominal Maximum Size* mm (in)		Minimum Mass g (lb)	
2.36	(No. 8)	10,000	(25)
4.75	(No. 4)	10,000	(25)
9.5	(3/8)	10,000	(25)
12.5	(1/2)	15,000	(35)
19.0	(3/4)	25,000	(55)
25.0	(1)	50,000	(110)
37.5	(1 1/2)	75,000	(165)
50	(2)	100,000	(220)
63	(2 1/2)	125,000	(275)
75	(3)	150,000	(330)
90	(3 1/2)	175,000	(385)

* One sieve larger than the first sieve to retain more than 10 percent of the material using an agency specified set of sieves based on cumulative percent retained. Where large gaps in specification sieves exist, intermediate sieve(s) may be inserted to determine nominal maximum size. Maximum size is one size larger than nominal maximum size.

Note 1: Based upon the tests required, the sample size may be four times that shown in Table 2 of the FOP for AASHTO T 27/T 11, if that mass is more appropriate. As a general rule the field sample size should be such that, when split twice will provide a testing sample of proper size.

Procedure – Specific Situations

• Conveyor Belts

Avoid sampling at the beginning or end of the aggregate run due to the potential for segregation. Be careful when sampling in the rain. Make sure to capture fines that may stick to the belt or that the rain tends to wash away.

Method A (From the Belt):

1. Stop the belt.
2. Set the sampling template in place on the belt, avoiding intrusion by adjacent material.
3. Scoop off the sample, including all fines.
4. Obtain a minimum of 3 increments.
5. Combine the increments to form a single sample.

Method B (From the Belt Discharge):

1. Pass a sampling device through the full stream of the material as it runs off the end of the conveyor belt. The sampling device may be manually, semi-automatic or automatically powered.
2. The sampling device shall pass through the stream at least twice, once in each direction, without overfilling while maintaining a constant speed during the sampling process.

3. When emptying the sampling device into the sample container, include all fines.
4. Combine the increments to form a single sample.

- **Transport Units**

1. Visually divide the unit into four quadrants.
2. Identify one sampling location in each quadrant.
3. Dig down and remove approximately 0.3 m (1 ft) of material to avoid surface segregation. Obtain each increment from below this level.
4. Combine the increments to form a single sample.

- **Roadways**

Method A (Berm or Windrow):

1. Sample prior to spreading.
2. Take the increments from a minimum of three random locations along the fully-formed windrow or berm. Do not take the increments from the beginning or the end of the windrow or berm.
3. Obtain full cross-section samples of approximately equal size at each location. Take care to exclude the underlying material.
4. Combine the increments to form a single sample.

Note 2: Sampling from berms or windrows may yield extra-large samples and may not be the preferred sampling location.

Method B (In-Place):

1. Sample after spreading and prior to compacting.
2. Take the increments from three random locations.
3. Obtain full-depth samples of approximately equal size from each location. Take care to exclude the underlying material.
4. Combine the increments to form a single sample.

- **Stockpiles**

Method A – Coarse, Fine, or a Combination of Coarse and Fine Aggregates:

1. Create, with a loader if one is available, horizontal surfaces with vertical faces in the top, middle, and bottom third of the stockpile. When no equipment is available a shovel may be used to create the horizontal surfaces with vertical faces.
2. Prevent continued sloughing by shoving a flat board in against the vertical face. Sloughed material will be discarded to create the horizontal surface.
3. Sample from the horizontal surface at the intersection of the horizontal and vertical faces.
4. Obtain at least one increment of equal size from each of the top, middle, and bottom thirds of the pile.

5. Combine the increments to form a single sample.

Method B – Fine Aggregate (Alternate Tube Method):

1. Remove the outer layer that may have become segregated.
2. Using a sampling tube, obtain one increment of equal size from a minimum of five random locations on the pile.
3. Combine the increments to form a single sample.

Note 3: Sampling at stockpiles should be avoided whenever possible due to problems involved in obtaining a representative gradation of material.

Addendum WAQTC FOP for AASHTO T 2

Following are guidelines for the use of WAQTC FOP for AASHTO T 2 by the State of Alaska DOT&PF.

1. Table 1, Minimum (Field) Sample Size, is modified to allow for reduced sample sizes in accordance with the Alaska DOT&PF Guidelines for WAQTC FOP for AASHTO T 27/T 11 (i.e. the field sample size is such that when split twice, it will provide a testing sample of proper size for WAQTC FOP for AASHTO T 27/T 11).

Table 1
Sample Sizes

Nominal Maximum Size *,		Minimum Mass,	
Standard	Alternate	kg	lb
mm	in		
2.36	No. 8	10	25
4.75	No. 4	10	25
9.5	3/8	10	25
12.5	1/2	15	35
19.0	3/4	25	55
25.0	1	45	100
37.5	1-1/2	65	145
50	2	85	190
75	3	125	275

*Nominal Maximum Size: One sieve larger than the first sieve to retain more than 10 percent of the material using an agency specified set of sieves based on cumulative percent retained. Where large gaps in specification sieves exist, intermediate sieve(s) may be inserted to determine nominal maximum size.

2. As an alternate to stockpile sampling Method A, use a loader to deposit a cross section of the stockpile in a pile, mix and distribute into a flattened miniature stockpile or pad 12 in to 18 in thick. Sample as indicated in Roadway Method B.

This page intentionally left blank.

REDUCING SAMPLES OF AGGREGATES TO TESTING SIZE

FOP FOR AASHTO T 248 (See Addendum for DOT&PF Guidelines)

Scope

This procedure covers the reduction of samples to the appropriate size for testing in accordance with AASHTO T 248. Techniques are used that minimize variations in characteristics between test samples and field samples. Method A (Mechanical Splitter) and Method B (Quartering) are covered.

This procedure applies to fine aggregate (FA), coarse aggregate (CA), and mixes of the two, and may also be used on soils.

Apparatus

Method A – Mechanical Splitter

Splitter chutes:

- Even number of equal width chutes
- Discharge alternately to each side
- Minimum of 8 chutes total for CA, 12 chutes total for FA
- Width:
 - Minimum 50 percent larger than largest particle
 - Maximum chute width of 19 mm (3/4 in.) for fine aggregate passing the 9.5 mm (3/8 in.) sieve

Feed control:

- Hopper or straightedge pan with a width equal to or slightly less than the overall width of the assembly of chutes
- Capable of feeding the splitter at a controlled rate

Splitter receptacles / pans:

- Capable of holding two halves of the sample following splitting

The splitter and accessory equipment shall be so designed that the sample will flow smoothly without restriction or loss of material.

Method B – Quartering

- Straightedge scoop, shovel, or trowel
- Broom or brush
- Canvas or plastic sheet, approximately 2 by 3 m (6 by 9 ft)

Method Selection

Samples of FA that are drier than the saturated surface dry (SSD) condition shall be reduced by a mechanical splitter according to Method A. As a quick determination, if the fine aggregate will retain its shape when molded with the hand, it is wetter than SSD.

Samples of FA that are at SSD or wetter than SSD shall be reduced by Method B, or the entire sample

may be dried to the SSD condition – using temperatures that do not exceed those specified for any of the tests contemplated – and then reduced to test sample size using Method A.


Samples of CA or mixtures of FA and CA may be reduced by either method. It may be undesirable to reduce some FA / CA mixtures that are over SSD condition using Method A.

Procedure

Method A – Mechanical Splitter

1. Place the sample in the hopper or pan and uniformly distribute it from edge to edge so that approximately equal amounts flow through each chute. The rate at which the sample is introduced shall be such as to allow free flowing through the chutes into the pans below.
2. Reduce the sample from one of the two pans as many times as necessary to reduce the sample to meet the minimum size specified for the intended test. The portion of the material collected in the other pan may be reserved for reduction in size for other tests. In lieu of the check for effective reduction in step 3, use the method illustrated in Figure 1.

Figure 1

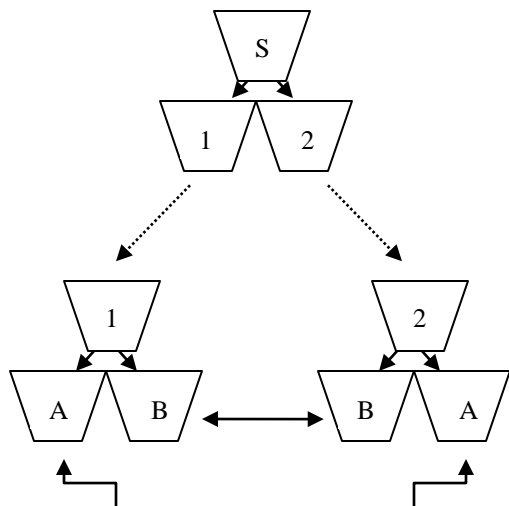

Sample (S) is an amount greater than or equal to twice the mass needed for testing. Sample (S) is reduced in a mechanical splitter to yield parts (1) and (2)

Part (1) is further reduced yielding (A) and (B) while part (2) is reduced to yield (B) and (A).

Final testing sample is produced by combining alternate pans, i.e. A/A or B/B only.

3. As a check for effective reduction, determine the mass of each reduced portion. If the percent difference of the two masses is greater than 5 percent, corrective action must be taken

Calculation

$$\frac{\text{Smaller Mass}}{\text{Larger Mass}} = \text{Ratio}$$

$$(1 - \text{Ratio}) \times 100 = \% \text{ Difference}$$

Procedure

Method B – Quartering

Use either of the following two procedures or a combination of both.

Procedure # 1: Quartering on a clean, hard, level surface:

1. Place the sample on a hard, clean, level surface where there will be neither loss of material nor the accidental addition of foreign material.
2. Mix the material thoroughly by turning the entire sample over a minimum of three times. With the last turning, shovel the entire sample into a conical pile by depositing each shovelful on top of the preceding one.
3. Flatten the conical pile to a uniform thickness and diameter by pressing down with a shovel. The diameter should be four to eight times the thickness.
4. Divide the flattened pile into four approximately equal quarters with a shovel or trowel.
5. Remove two diagonally opposite quarters, including all fine material, and brush the cleared spaces clean.
6. Successively mix and quarter the remaining material until the sample is reduced to the desired size.
7. The final test sample consists of two diagonally opposite quarters.

Procedure # 2: Quartering on a canvas or plastic sheet:

1. Place the sample on the sheet.
2. Mix the material thoroughly a minimum of four times by pulling each corner of the sheet horizontally over the sample toward the opposite corner. After the last turn, form a conical pile.
3. Flatten the conical pile to a uniform thickness and diameter by pressing down with a shovel. The diameter should be four to eight times the thickness.
4. Divide the flattened pile into four approximately equal quarters with a shovel or trowel, or, insert a stick or pipe beneath the sheet and under the center of the pile, then lift both ends of the stick, dividing the sample into two roughly equal parts. Remove the stick leaving a fold of the sheet between the divided portions. Insert the stick under the center of the pile at right angles to the first division and again lift both ends of the stick, dividing the sample into four roughly equal quarters.
5. Remove two diagonally opposite quarters, being careful to clean the fines from the sheet.
6. Successively mix and quarter the remaining material until the sample size is reduced to the desired size.
7. The final test sample consists of two diagonally opposite quarters.

Addendum WAQTC FOP for AASHTO T 248

Following are guidelines for the use of WAQTC FOP for AASHTO T 248 by the State of Alaska DOT&PF.

1. When determining the correct number of chutes, the chutes will be a minimum of 50 percent larger than the largest particle, utilizing the maximum number of chutes possible.
2. AASHTO T 248 Method C may be used.

SIEVE ANALYSIS OF FINE AND COARSE AGGREGATES

FOP FOR AASHTO T 27 (See Addendum for DOT&PF Guidelines)

MATERIALS FINER THAN 75- μ m (No. 200) SIEVE IN MINERAL AGGREGATE BY WASHING (See Addendum for DOT&PF Guidelines)

FOP FOR AASHTO T 11

Scope

Sieve analysis determines the gradation or distribution of aggregate particle sizes within a given sample.

Accurate determination of material smaller than 75 μ m (No. 200) cannot be made with AASHTO T 27 alone. If quantifying this material is required, it is recommended that AASHTO T 27 be used in conjunction with AASHTO T 11.

This FOP covers sieve analysis in accordance with AASHTO T 27 and materials finer than 75 μ m (No. 200) in accordance with AASHTO T 11 performed in conjunction with AASHTO T 27. The procedure includes three method choices: A, B, and C.

Apparatus

- Balance or scale: Capacity sufficient for the masses shown in Table 2, accurate to 0.1 percent of the sample mass or readable to 0.1 g, and meeting the requirements of AASHTO M 231
- Sieves: Meeting the requirements of AASHTO M 92
- Mechanical sieve shaker: Meeting the requirements of AASHTO T 27
- Suitable drying equipment (see FOP for AASHTO T 255)
- Containers and utensils: A pan or vessel of a size sufficient to contain the sample covered with water and to permit vigorous agitation without loss of any part of the sample or water
- Optional mechanical washing device

Sample Sieving

In all procedures, it is required to shake the sample over nested sieves. Sieves are selected to furnish information required by specification. The sieves are nested in order of decreasing size from the top to the bottom and the sample, or a portion of the sample, is placed on the top sieve.

Sieves are shaken in a mechanical shaker for approximately 10 minutes, or the minimum time determined to provide complete separation for the sieve shaker being used.

Time Evaluation

The minimum time requirement should be evaluated for each shaker at least annually by the following method: Continue shaking for a sufficient period and in such a manner that, after completion, not more than 0.5 percent by mass of the total sample passes any sieve during one minute of continuous hand sieving.

Provide a snug-fitting pan and cover, and hold in a slightly inclined position in one hand. Strike the side of the sieve sharply and with an upward motion against the heel of the other hand at the rate of about 150 times per minute, turning the sieve about one sixth of a revolution at intervals of about 25 strokes. In determining sufficiency of sieving for sizes larger than 4.75 mm (No. 4), limit the material on the sieve to a single layer of particles.

Overload Determination

Additional sieves may be necessary to provide other information, such as fineness modulus, or to keep from overloading sieves. The sample may also be sieved in increments. For sieves with openings smaller than 4.75 mm (No. 4), the mass retained on any sieve shall not exceed 7 kg/m² (4 g/in²) of sieving surface area. For sieves with openings 4.75 mm (No. 4) and larger, the mass, in grams shall not exceed the product of 2500 x (sieve opening in mm) x (sieving area in m²). See Table 1.

TABLE 1
Maximum Allowable Mass of Material Retained on a Sieve, g
Nominal Sieve Size, mm (in.)
Exact size is smaller (see AASHTO T 27)

Sieve Size mm (in.)		203 ϕ (8)	305 ϕ (12)	305 x 305 (12 x 12)	350 x 350 (14 x 14)	372 x 580 (16 x 24)
		Sieving Area m ²				
		0.0285	0.0670	0.0929	0.1225	0.2158
90	(3 1/2)	*	15,100	20,900	27,600	48,500
75	(3)	*	12,600	17,400	23,000	40,500
63	(2 1/2)	*	10,600	14,600	19,300	34,000
50	(2)	3600	8400	11,600	15,300	27,000
37.5	(1 1/2)	2700	6300	8700	11,500	20,200
25.0	(1)	1800	4200	5800	7700	13,500
19.0	(3/4)	1400	3200	4400	5800	10,200
16.0	(5/8)	1100	2700	3700	4900	8600
12.5	(1/2)	890	2100	2900	3800	6700
9.5	(3/8)	670	1600	2200	2900	5100
6.3	(1/4)	440	1100	1500	1900	3400
4.75	(No. 4)	330	800	1100	1500	2600
-4.75	(-No. 4)	200	470	650	860	1510

Sample Preparation

Obtain samples in accordance with the FOP for AASHTO T 2 and reduce to the size shown in Table 2 in accordance with the FOP for AASHTO T 248. These sample sizes are standard for aggregate testing but, due to equipment restraints, samples may need to be partitioned into several “subsamples.” For example, a gradation that requires 100,000 g (220 lbs) of material would not fit into a large tray shaker in one batch.

Some agencies permit reduced sample sizes if it is proven that doing so is not detrimental to the test results. Some agencies require larger sample sizes. Check agency guidelines for required or permitted test sample sizes.

TABLE 2
Sample Sizes for Aggregate Gradation Test

Nominal Maximum Size* mm (in.)		Minimum Dry Mass g (lb)	
4.75	(No. 4)	500	(1)
6.3	(1/4)	1,000	(2)
9.5	(3/8)	1,000	(2)
12.5	(1/2)	2,000	(4)
19.0	(3/4)	5,000	(11)
25.0	(1)	10,000	(22)
37.5	(1 1/2)	15,000	(33)
50	(2)	20,000	(44)
63	(2 1/2)	35,000	(77)
75	(3)	60,000	(130)
90	(3 1/2)	100,000	(220)
100	(4)	150,000	(330)
125	(5)	300,000	(660)

**Nominal maximum size: One sieve larger than the first sieve to retain more than 10 percent of the material using an agency specified set of sieves based on cumulative percent retained. Where large gaps between specification sieves exist, intermediate sieve(s) may be inserted to determine nominal maximum size.*

Selection of Procedure

Agencies may specify what method will be performed. If a method is not specified method A will be performed.

Overview

Method A

- Determine dry mass of original sample
- Wash through a 75µm (No. 200) sieve
- Determine dry mass of washed sample
- Sieve material

Method B

- Determine dry mass of original sample
- Wash through a 75µm (No. 200) sieve
- Determine dry mass of washed sample
- Sieve coarse material
- Determine mass of fine material
- Reduce fine portion
- Determine mass of reduced portion
- Sieve fine portion

Method C

- Determine dry mass of original sample
- Sieve coarse material
- Determine mass of fine material
- Reduce fine portion
- Determine mass of reduced portion
- Wash through a 75µm (No. 200) sieve
- Determine dry mass of washed sample
- Sieve reduced fine portion

Procedure Method A

1. Dry the sample to a constant mass in accordance with the FOP for AASHTO T 255, and record to the nearest 0.1 percent of the total sample mass or 0.1 g.
2. When the specification requires that the amount of material finer than 75 µm (No. 200) be determined, perform Step 3 through Step 9; otherwise, skip to Step 10.
3. Nest a sieve, such as a 2.0 mm (No. 10), above the 75 µm (No. 200) sieve.
4. Place the test sample in a container and add sufficient water to cover it.

Note 1: A detergent, dispersing agent, or other wetting solution may be added initially to the water to assure a thorough separation of the material finer than the 75 µm (No. 200) sieve from the coarser particles. There should be enough wetting agent to produce a small amount of suds when the sample is agitated. Excessive suds may overflow the sieves and carry material away with them.

5. Agitate vigorously to ensure complete separation of the material finer than 75 µm (No. 200) from coarser particles and bring the fine material into suspension above the coarser material. When using a mechanical washing device, exercise caution to avoid degradation of the sample.
6. Immediately pour the wash water containing the suspended and dissolved solids over the nested sieves, being careful not to pour out the coarser particles.
7. Add a second change of water to the sample remaining in the container, agitate, and repeat Step 6. Repeat the operation until the wash water is reasonably clear. If a detergent or dispersing agent is used, continue washing until the agent is removed.
8. Remove the upper sieve and rinse the material retained on the 75 µm (No. 200) sieve until water passing through the sieve is reasonably clear.
9. Return all material retained on the nested sieves to the container by flushing into the washed sample.

Note 2: Excess water may be carefully removed with a bulb syringe as long as the removed water is discharged back over the No. 200 sieve to preclude loss of fines.

10. Dry the washed aggregate to constant mass in accordance with the FOP for AASHTO T 255, and then cool prior to sieving. Record the “dry mass after washing”.
11. Select sieves to furnish the information required by the specifications. Nest the sieves in order of decreasing size from top to bottom and place the sample, or a portion of the sample, on the top sieve.
12. Place sieves in mechanical shaker and shake for the minimum time determined to provide complete separation for the sieve shaker being used (approximately 10 minutes).

Note 3: Excessive shaking (more than 10 minutes) may result in degradation of the sample.

13. Determine the individual or cumulative mass retained on each sieve and the pan to the nearest 0.1 percent or 0.1 g. Ensure that all material trapped in the openings of the sieve are cleaned out and included in the mass retained.

Note 4: Use coarse wire brushes to clean the 600 µm (No. 30) and larger sieves, and soft bristle brushes for smaller sieves.

14. In the case of coarse / fine aggregate mixtures, the minus 4.75 mm (No. 4) may be distributed among two or more sets of sieves to prevent overloading of individual sieves.

Calculations

The total mass of the material after sieving, for both coarse and fine portions should check closely with the original mass of sample placed on the sieves. If performing T 11 with T 27, this would be the dry mass after wash. If performing just T 27 this would be the original dry mass. When the masses before and after sieving differ by more than 0.3 percent, do not use the results for acceptance purposes.

Calculate the total percentages passing, individual or cumulative percentages retained, or percentages in various size fractions to the nearest 0.1 percent by dividing the masses for Method A, or adjusted masses for methods B and C, on the individual sieve masses or cumulative sieve masses by the total mass of the initial dry sample. If the same test sample was first tested by T 11, use the total dry sample mass prior to washing in T 11 as the basis for calculating all percentages. Report percent passing as indicated in the “Report” section at the end of this FOP.

Percent Retained:

Where:

IPR= Individual Percent Retained

CPR= Cumulative Percent Retained

M= Total Dry Sample mass before washing

IMR= Individual Mass Retained OR Adjusted Individual mass from Methods B or C

CMR= Cumulative Mass Retained OR Adjusted Cumulative Mass from Methods B or C

$$IPR = \frac{IMR}{M} \times 100 \quad \text{OR} \quad CPR = \frac{CMR}{M} \times 100$$

Percent Passing (Calculated):

Where:

PP= Percent Passing

PPP= Previous Percent Passing

$$PP = PPP - IPR \quad \text{OR} \quad PP = 100 - CPR$$

Procedure Method B

1. Perform steps 1 through 10 from the “Procedure – Method A”, then continue as follows:
2. Select sieves to furnish information required by the specifications. Nest the sieves in order of decreasing size from top to bottom through the 4.75 mm (No. 4) with a pan at the bottom to retain the minus 4.75 mm (No. 4).
3. Place the sample, or a portion of the sample, on the top sieve. Sieves may already be in the mechanical shaker, or place the sieves in the mechanical shaker and shake for the minimum time determined to provide complete separation for the sieve shaker being used (approximately 10 minutes).

Note 3: Excessive shaking (more than 10 minutes) may result in degradation of the sample.

4. Determine the individual or cumulative mass retained on each sieve to the nearest 0.1 percent or 0.1 g. Ensure that all particles trapped in the openings of the sieve are cleaned out and included in the mass retained.

Note 4: Use coarse wire brushes to clean the 600 µm (No. 30) and larger sieves, and soft hair bristle for smaller sieves.

5. Determine the mass of the material in the pan [minus 4.75 mm (No. 4)] (M_1).
6. Reduce the minus 4.75 mm (No. 4) using a mechanical splitter in accordance with the FOP for AASHTO T 248 to produce a sample with a mass of 500 g minimum. Determine and record the mass of the minus 4.75 mm (No. 4) split (M_2).
7. Select fine sieves to furnish information required by the specifications. Nest the sieves in order of decreasing size from top to bottom through the 75 µm (No. 200) with a pan at the bottom to retain the minus 75µm (No. 200).
8. Repeat steps 3 and 4, Method B, with the minus 4.75 mm (No. 4) including determining the mass of the material in the pan.
- 9a. Compute the “Adjusted Individual Mass Retained” of the size increment of the original sample as follows when determining “Individual Mass Retained”.

$$IMR = \frac{M_1}{M_2} \times B$$

where:

IMR = adjusted individual mass retained of the size increment on a total sample basis

M_1 = mass of minus 4.75mm (No. 4) sieve in total sample

M_2 = mass of minus 4.75mm (No. 4) sieve actually sieved

B = individual mass of the size increment in the reduced portion sieved

- 9b. Compute the “Adjusted Cumulative Mass Retained” of the size increment of the original sample as follows when determining “Cumulative Mass Retained”:

$$\text{CMR} = \left(\frac{M_1}{M_2} \times B \right) + D$$

where:

CMR = Total cumulative mass retained of the size increment based on a total sample

M_1 = mass of minus 4.75mm (No. 4) sieve in total sample

M_2 = mass of minus 4.75mm (No. 4) sieve actually sieved

B = cumulative mass of the size increment in the reduced portion sieved

D = cumulative mass of plus 4.75mm (No. 4) portion of sample

- 9c. For Percent Passing (Calculated) see “Calculation” under Method A.

Procedure Method C

1. Dry sample in accordance with the FOP for AASHTO T 255. Determine and record the total dry mass of the sample to the nearest 0.1 percent.
Note 6: AASHTO T 27 allows for coarse aggregate to be run in a moist condition unless the nominal maximum size of the aggregate is smaller than 12.5 mm (1/2 in.), the coarse aggregate (CA) contains appreciable material finer than 4.75 mm (No. 4), or the coarse aggregate is highly absorptive.
2. Break up any aggregations or lumps of clay, silt or adhering fines to pass the 4.75 mm (No. 4) sieve. If substantial coatings remain on the coarse particles in amounts that would affect the percent passing any of the specification sieves, the sample should be tested with either Method A or Method B.
3. Select sieves to furnish information required by the specifications. Nest the sieves in order of decreasing size from top to bottom through the 4.75 mm (No.4) with a pan at the bottom to retain the minus 4.75 mm (No. 4).
4. Place the sample, or a portion of the sample, on the top sieve. Sieves may already be in the mechanical shaker or place the sieves in the mechanical shaker and shake for the minimum time determined to provide complete separation for the sieve shaker being used (approximately 10 minutes).

Note 3: Excessive shaking (more than 10 minutes) may result in degradation of the sample.

5. Determine the individual or cumulative mass retained on each sieve to the nearest 0.1 percent or 0.1 g. Ensure that all material trapped in the openings of the sieve are cleaned out and included in the mass retained.

Note 4: Use coarse wire brushes to clean the 600 μ m (No. 30) and larger sieves, and soft bristle brush for smaller sieves.

6. Determine the mass of material in the pan [minus 4.75 mm (No. 4)] (M_1).
7. Reduce the minus 4.75mm (No. 4), using a mechanical splitter in accordance with the FOP for AASHTO T 248, to produce a sample with a mass of 500 g minimum.
8. Determine and record the mass of the minus 4.75mm (No. 4) split (M_3).

9. Perform steps 3 through 10 of Method A (Wash) on the minus 4.75mm (No. 4) split.
10. Select fine sieves to furnish information required by the specifications. Nest the sieves in order of decreasing size from top to bottom through the 75µm (No. 200) with a pan at the bottom to retain the minus 75 µm (No. 200).
11. Repeat steps 4 and 5, Method C, with the minus 4.75mm (No. 4) including determining the mass of the material in the pan.
- 12a. Compute the “Adjusted Individual Mass Retained” of the size increment of the original sample as follows when determining “Individual Mass Retained”:

where:

$$IMR = \frac{M_1}{M_3} \times B$$

IMR = adjusted individual mass of the size increment on a total sample basis

M_1 = mass of the minus 4.75mm (No. 4) sieve in total sample

M_3 = mass of reduced portion of the minus 4.75mm (No. 4) before washing

B = mass of the size increment in the reduced portion sieved

- 12b. Compute the “Adjusted Cumulative Mass Retained” of the size increment of the original sample as follows when determining “Cumulative Mass Retained”:

$$CMR = \left(\frac{M_1}{M_3} \times B \right) + D$$

where:

CMR = total cumulative mass of the size increment based on a total sample

M_1 = mass of fraction finer than 4.75mm (No. 4) sieve in total sample

M_3 = mass of reduced portion of material finer than 4.75mm (No. 4) before washing

B = cumulative mass of the size increment in the reduced portion sieved

D = cumulative mass of plus 4.75mm (No. 4) portion of sample

- 12c. For Percent Passing (Calculated) see “Calculation” under Method A.

Fineness Modulus

Fineness Modulus (FM) is used in determining the degree of uniformity of the aggregate gradation in PCC mix designs. It is an empirical number relating to the fineness of the aggregate. The higher the FM, the coarser the aggregate. Values of 2.40 to 3.00 are common for FA in PCC.

The sum of the cumulative percentages retained on the sieves in the following table divided by 100 gives the FM.

Required Sieves and Sample Calculation

	Example A				Example B		
	Percent				Percent		
		Retained				Retained	
Sieve Size mm (in)	Passing		On Spec'd Sieves*		Passing		On Spec'd Sieves*
75 (3)	100	0	0		100	0	0
37.5 (1 1/2)	100	0	0		100	0	0
19 (3/4)	15	85	85		100	0	0
9.5 (3/8)	0	100	100		100	0	0
4.75 (No.4)	0	100	100		100	0	0
2.36 (No.8)	0	100	100		87	13	13
1.18 (No.16)	0	100	100		69	31	31
0.60 (No.30)	0	100	100		44	56	56
0.30 (No.50)	0	100	100		18	82	82
0.15 (No. 100)	0	100	100		4	96	96
			$\Sigma = 785$				$\Sigma = 278$
			FM = 7.85				FM = 2.78

In decreasing size order, each sieve is one-half the size of the preceding sieve.

Report

Results shall be reported on standard forms approved for use by the agency. Depending on the agency, this may include:

- Mass retained on each sieve
- Percent retained on each sieve
- Cumulative mass retained on each sieve
- Cumulative percent retained on each sieve
- Percent passing each sieve to the nearest 1 percent except for the percent passing the 75 μm (No. 200) sieve, which shall be reported to the nearest 0.1 percent
- FM to the nearest 0.01

Addendum WAQTC FOP for AASHTO T 27/T 11

Following are guidelines for the use of WAQTC FOP for AASHTO T 27/T 11 by the State of Alaska DOT&PF.

1. Delete Table 2 and replace with Table 3:

Table 3
Sample sizes for Aggregate Sieve Analysis

Nominal Maximum Size*		Minimum Mass	
Standard	Alternate		
mm	in	kg	lb
4.75	No. 4	0.5	1
6.3	1/4	1	2
9.5	3/8	1	2
12.5	1/2	2	4
19.0	3/4	5	11
25.0	1	10	22
37.5	1-1/2	15	33
50	2	20	44
75	3	30	66

*Nominal Maximum size: One sieve larger than the first sieve to retain more than 10 percent of the material using an agency specified set of sieves based on cumulative percent retained. Where large gaps between specification sieves exist, intermediate sieve(s) may be inserted to determine nominal maximum size.

2. AKDOT&PF does not allow the coarse aggregate to be run in a moist condition for sieve analysis.
3. Unless otherwise specified, Method C shall be used.
4. For calculating Fineness Modulus, subtract reported percent passing from 100 to determine percent retained.
5. The following alternate method of calculation can be used for Method C.

Example given:

Dry Mass of total sample: $M = 3304.5$ g

Dry Mass of minus 4.75mm (No. 4) reduced portion before wash: $M_{\#4} = 527.6$

Dry Mass of minus 4.75mm (No. 4) reduced portion after wash: 495.3

$$CPR = \frac{(CMR)}{M} \times 100 \qquad CPP = 100 - CPR$$

Also: $CPP = 100 \times (M - CMR) / M$

Gradation on Coarse Sieves

Sieve Size mm (in.)	Cumulative Mass Retained, g (CMR)	Cal'd Percent Retained (CPR)	Cal'd Percent Passing (CPP)	Reported Percent Passing* (RPP)
16.0 (5/8)	0	0.0	100.0	100
12.5 (1/2)	125.9	3.8	96.2	96
9.50 (3/8)	604.1	18.3	81.7	82
4.75 (No. 4)	1295.6	39.2	60.8	61
Pan	2008.9			
Total Dry Sample = 3304.5				

Coarse check sum: $[(3304.5 - 3304.5) / 3304.5] \times 100 = 0.0\%$ is within the 0.3 percent requirement

For Percent Passing (Calculated) see "Calculation" under Method A

Note 4: The pan mass determined in the laboratory and the calculated mass ($3304.5 - 1295.6 = 2008.9$) should be the same if no material was lost.

The pan (2008.9 g) was reduced in accordance with the FOP for AASHTO T 248, so that at least 500 g are available. In this case, the mass determined was $M_{\#4} = 527.6$ g.

$$CPR_{\#4} = \frac{CMR_{\#4}}{M_{\#4}} \times 100 \quad CPP_{\#4} = 100 - CPR_{\#4} \quad CPP = \left(CPP_{\#4} \times CPP_{\#4} \right) \div 100$$

Where:

$CMR_{\#4}$ = Cumulative mass retained for the sieve size based on a -#4 split sample

$CPR_{\#4}$ = Calculated percent retained based on the -#4 split

$CPP_{\#4}$ = Calculated percent passing based on the -#4 split

$M_{\#4}$ = Total mass of the -#4 split before washing.

$CPP_{\#4}$ = Calculated percent passing the #4 sieve.

**Final Gradation on All Sieves
Calculation by Individual Mass**

Sieve Size mm (in.)	Cumulative Mass Retained, g (CMR _{#4})	Cal'd Percent Retained _{#4} (CPR _{#4})	Cal'd Percent Passing _{#4} (CPP _{#4})	Cal'd Percent Passing (CPP)	Reported Percent Passing* (RPP)
16.0 (5/8)				100.0	100
12.5 (1/2)	Coarse sieve information on previous page.			96.2	96
9.5 (3/8)				81.7	82
4.75 (No. 4)				60.8	61
2.0 (No. 10)	194.3	36.8	63.2	38.4	38
0.425 (No. 40)	365.6	69.3	30.7	18.7	19
0.210 (No. 80)	430.8	81.7	18.3	11.1	11
0.075 (No. 200)	484.4	91.8	8.2	5.0	5.0
Pan	495.1				
Dry mass (M _{D before wash}) of minus 4.75 mm (No. 4) sample, before washing: 527.6 g					
Dry mass of minus 4.75 mm (No. 4) sample, after washing: 495.3 g					

*Report 75 µm (No. 200) sieve to 0.1 percent. Report all others to 1 percent

Fine check sum: $[(495.3 - 495.1) / 495.3] \times 100 = 0.04\%$ is within the 0.3 percent requirement.

Also note that for Minus #4 material using this method that:

$$CPP = CPP_{\#4} \times (M_{D \text{ before wash}} - CMR_{\#4}) / M_{D \text{ before wash}}$$

DETERMINING THE PERCENTAGE OF FRACTURE IN COARSE AGGREGATE FOP FOR AASHTO T 335

Scope

This procedure covers the determination of the percentage, by mass, of a coarse aggregate (CA) sample that consists of fractured particles meeting specified requirements in accordance with AASHTO T 335.

In this procedure, a sample of aggregate is screened on the sieve separating CA and fine aggregate (FA). This sieve will be identified in the agency's specifications, but might be the 4.75 mm (No. 4) sieve. The CA particles are visually evaluated to determine conformance to the specified fracture. The percentage of conforming particles, by mass, is calculated for comparison to the specifications.

Apparatus

- Balance or scale: Capacity sufficient for the principle sample mass, accurate to 0.1 percent of the sample mass or readable to 0.1 g, and meeting the requirements of AASHTO M 231.
- Sieves: Meeting requirements of AASHTO M 92.
- Splitter: Meeting the requirements of FOP for AASHTO T 248.

Terminology

1. Fractured Face: An angular, rough, or broken surface of an aggregate particle created by crushing or by other means. A face is considered a "fractured face" whenever one-half or more of the projected area, when viewed normal to that face, is fractured with sharp and well defined edges. This excludes small nicks.
2. Fractured particle: A particle of aggregate having at least the minimum number of fractured faces specified. (This is usually one or two.)

Sampling and Sample Preparation

1. Sample and reduce the aggregate in accordance with the FOPs for AASHTO T 2 and T 248.
2. When the specifications list only a total fracture percentage, the sample shall be prepared in accordance with Method 1. When the specifications require that the fracture be counted and reported on each sieve, the sample shall be prepared in accordance with Method 2.
3. Method 1 - Combined Fracture Determination
 - a. Dry the sample sufficiently to obtain a clean separation of FA and CA material in the sieving operation.
 - b. Sieve the sample in accordance with the FOP for AASHTO T 27/T 11 over the 4.75 mm (No. 4) sieve, or the appropriate sieve listed in the agency's specifications for this material.

Note 1: Where necessary, wash the sample over the sieve or sieves designated for the determination of fractured particles to remove any remaining fine material, and dry to a constant mass in accordance with the FOP for AASHTO T 255.

- c. Reduce the sample using Method A – Mechanical Splitter, in accordance with the FOP for AASHTO T 248, to the appropriate test size. This test size should be slightly larger than shown in Table 1, to account for loss of fines through washing if necessary.

TABLE 1
Sample Size
Method 1 (Combined Sieve Fracture)

Nominal Maximum Size* mm (in.)	Minimum Sample Mass Retained on 4.75 mm (No. 4) Sieve g (lb)
37.5 (1 1/2)	2500 (6)
25.0 (1)	1500 (3.5)
19.0 (3/4)	1000 (2.5)
12.5 (1/2)	700 (1.5)
9.5 (3/8)	400 (0.9)
4.75 (No. 4)	200 (0.4)

* One sieve larger than the first sieve to retain more than 10 percent of the material using an agency specified set of sieves based on cumulative percent retained. Where large gaps in specification sieves exist, intermediate sieve(s) may be inserted to determine nominal maximum size.

4. Method 2 – Individual Sieve Fracture Determination

- a. Dry the sample sufficiently to obtain a clean separation of FA and CA material in the sieving operation. A washed sample from the gradation determination (the FOP for T 27/T 11) may be used.
- b. If not, sieve the sample in accordance with the FOP for AASHTO T 27/T 11 over the sieves listed in the specifications for this material.

Note 2: If overload (buffer) sieves are used the material from that sieve must be added to the next specification sieve.

- c. The size of test sample for each sieve shall meet the minimum size shown in Table 2. Utilize the total retained sieve mass or select a representative portion from each sieve mass by splitting or quartering in accordance with the FOP for AASHTO T 248.

Note 1: Where necessary, wash the sample over the sieve or sieves designated for the determination of fractured particles to remove any remaining fine material, and dry to a constant mass in accordance with the FOP for AASHTO T 255.

TABLE 2
Sample Size
Method 2 (Individual Sieve Fracture)

Sieve Size mm (in.)		Minimum Sample Mass g (lb)	
31.5	(1 1/4)	1500	(3.5)
25.0	(1)	1000	(2.2)
19.0	(3/4)	700	(1.5)
16.0	(5/8)	500	(1.0)
12.5	(1/2)	300	(0.7)
9.5	(3/8)	200	(0.5)
6.3	(1/4)	100	(0.2)
4.75	(No. 4)	100	(0.2)
2.36	(No. 8)	25	(0.1)
2.00	(No. 10)	25	(0.1)

Note 3: If fracture is determined on a sample obtained for gradation, use the mass retained on the individual sieves, even if it is less than the minimum listed in Table 2. If less than 5 percent of the total mass is retained on a single specification sieve, include that material on the next smaller specification sieve. If a smaller specification sieve does not exist, this material shall not be included in the fracture determination.

Procedure

1. After cooling, spread the dried sample on a clean, flat surface large enough to permit careful inspection of each particle. To verify that a particle meets the fracture criteria, hold the aggregate particle so that the face is viewed directly.
2. To aid in making the fracture determination, separate the sample into three categories:
 - fractured particles meeting the criteria
 - particles not meeting the criteria
 - questionable or borderline particles
3. Determine the dry mass of particles in each category to the nearest 0.1 g.
4. If, on any determination, more than 15 percent of the total mass of the sample is placed in the questionable category, repeat the sorting procedure until no more than 15 percent is present in that category.

Calculation

Calculate the mass percentage of questionable fractured particles to the nearest 1 percent using the following formula:

$$\%Q = \frac{Q}{(F + Q + N)} \times 100$$

where: % Q = Percent of questionable fractured particles
 F = Mass of fractured particles
 Q = Mass of questionable or borderline particles
 N = Mass of unfractured particles

Calculate the mass percentage of fractured faces to the nearest 1 percent using the following formula:

$$P = \frac{\left(\frac{Q}{2} + F\right)}{(F + Q + N)} \times 100$$

where: P = Percent of fracture
 F = Mass of fractured particles
 Q = Mass of questionable or borderline particles
 N = Mass of unfractured particles

Report

Results shall be reported on standard forms approved for use by the agency. Report fracture to the nearest 1 percent.

Addendum WAQTC FOP for AASHTO 335

Following are guidelines for the use of WAQTC FOP for AASHTO T 335 by the State of Alaska DOT&PF.

1. Fracture is determined on the + No. 4 material unless otherwise specified.

This page intentionally left blank.

Determining the Percentage of Flat and Elongated Particles in Coarse Aggregate ATM 306

1. Scope

This procedure covers the determination of the percentages of flat (thin) and elongated particles in coarse aggregates.

2. Apparatus

The apparatus used shall consist of any suitable equipment, by means of which aggregate particles may be tested for compliance, at the dimensional ratios desired, with the definitions given below. Types of acceptable apparatus are:

- ASTM Proportional Caliper Device meeting the requirements of ASTM D 4791. Illustrated in Figure 1.
- Balance or scale: Capacity sufficient for the principle sample mass, readable 0.1 percent or 0.1 g and meeting the requirements of AASHTO M 231.

Note: For this test, this would require a scale with a capacity of at least 1200 g and readable to 0.1 g, or better.

- Sieves, meeting the requirements of AASHTO M 92.

3. Definitions

1. Length — maximum dimension of the particle.
2. Thickness — maximum dimension perpendicular to the length and width.
3. Flat ("Thin") & Elongated Particle — a particle having a ratio of length to thickness greater than that specified.

4. Sampling and Sample Preparation

1. Sample and reduce the aggregate in accordance with the FOPs for AASHTO T 2 and T 248.
2. Flat and Elongated Determination
 - a. Dry the sample sufficiently to obtain a clean separation of FA and CA material in the sieving operation.
 - b. Sieve the sample in accordance with the FOP for AASHTO T 27/ T 11 over the 4.75 mm (No. 4) sieve.
 - c. Reduce the sample using Method A – Mechanical Splitter, in accordance with the FOP for AASHTO T 248, to the appropriate test size. This test size should be slightly larger than shown in Table 1, to account for loss of fines through washing if necessary.

Table 1
Sample Size

Size Fraction		Minimum Sample Mass
(mm)	(in)	g
37.5 to 19.0	1½ to ¾	1000
19.0 to 9.5	¾ to ⅜	500
9.5 to 4.75	⅜ to No. 4	100

Note 1: If this test is performed using a sample obtained for gradation, use the mass retained for the size fraction, regardless of the sample mass required by Table 1. If less than 5 percent of the total mass is retained on a single specification sieve, include that material on the next smaller specification sieve.

5. Procedure

1. Unless specified, the caliper ratio shall be 1:5.
2. Determine and record the total dry mass of the size grouping to be tested to the nearest 0.1g.
3. Flat and Elongated Particle Test — Recombine, if necessary, all of the particles from the above process.
4. Set the larger opening to the particle's length. The particle is flat and elongated if the particle's thickness can pass completely through the smaller opening.
5. Determine and record the mass of the flat and elongated particles to the nearest 0.1 g.

6. Calculation

1. Calculate the cumulative percent retained.

$$CPR = (100 - CPP)$$

Where :

CPR = Cumulative percent retained on original sample gradation

CPP = Cumulative percent passing from original sample gradation.

2. Calculate the cumulative percent retained of each size group in relation to the total plus 4.75 mm (No. 4).

$$\text{FnE Group IMR} = \text{FnE Group CPR} - \text{Next Larger Group CPR}$$

3. Calculate the individual percent retained of each size.

$$\text{FnE Group IMR} = \text{FnE Group CPR} - \text{Next Larger Group CPR}$$

4. Calculate the percent flat and elongated (FnE) for each size group.

$$\% \text{ F \& E for Size Group} = [(\text{Mass FnE Size Group}) / (\text{Size Group Mass})] \times 100$$

6. Calculate the weighted percent for each size.

Weighted % FnE Size Group = % F & E for Size Group \times FnE Group IPR

7. Calculate the total percentage of FnE by determining the sum of all the weighted % FnE for Size Groups.

7. Report

Report the required data on Department forms to the nearest whole percent.

ASTM Proportional Caliper
Figure 1



Caliper set to 1:5 ratio



Length Determination

Thin (Flat) Determination

This page intentionally left blank.



STATE OF ALASKA
DOT & PF

AGGREGATE, Sand Equivalent
FIELD WORKSHEET

☐ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____ AKSAS No: _____

Material: _____ Source: _____

Item No: _____ Location: _____

Sta. / Sampled from: _____ Sampled by: _____

C_L & Grade Reference: _____ Qualification No: _____ Date Sampled: _____

Sand Equivalent WAQTC FOP T 176			
Sedimentation Time		20 min.	
Trial No.	1	2	3
Sand Reading SR			
Clay Reading CR			
Sand Equivalent SE			
Sedimentation Time			
SE = (SR / CR) * 100			
Test by/date:		Average	

Flat and Elongated ATM 306								
Ratio: <input type="checkbox"/> 1:5 <input type="checkbox"/> 1:3 <input type="checkbox"/> 1:2								
Size Group mm — in	% Pass Original (CPP)	% Ret. Origin = (100-CPP)	FnE Group CPR	FnE Group IPR	Size Group Mass	Mass FnE Size Group	% FnE Size Group (B)	Weighted % FnE Size Group
37.5 to 19.0	1½ to ¾							
19 to 9.5	¾ to ⅜							
9.5 to 4.75	⅜ to No. 4							
FnE Group CPR = (Smallest Sieve in Group %Ret. ÷ % No. 4 Retained) × 100						Total Weighted %		
FnE Group IMR = FnE Group CPR - Next Larger Group CPR								
% F & E Size Group (B) = [(Mass FnE Size Group) / (Size Group Mass)] * 100						Test by/date:		
Weighted FnE Size Group = B × FnE Group IPR								

Remarks: _____

Signature / Date: _____

Checked by / Date: _____

PLASTIC FINES IN GRADED AGGREGATES AND SOILS BY THE USE OF THE SAND EQUIVALENT TEST

WAQTC FOP FOR AASHTO T 176

Scope

This procedure covers the determination of plastic fines in accordance with AASHTO T 176. It serves as a rapid test to show the relative proportion of fine dust or clay-like materials in fine aggregates (FA) and soils.

Apparatus

See AASHTO T 176 for a detailed listing of sand equivalent apparatus. Note that the siphon tube and blow tube may be glass or stainless steel as well as copper.

- Graduated plastic cylinder.
- Rubber stopper.
- Irrigator tube.
- Weighted foot assembly: Having a mass of $1000 \pm 5\text{g}$. There are two models of the weighted foot assembly. The older model has a guide cap that fits over the upper end of the graduated cylinder and centers the rod in the cylinder. It is read using a slot in the centering screws. The newer model has a sand-reading indicator 254 mm (10 in.) above this point and is preferred for testing clay-like materials.
- Siphon assembly: The siphon assembly will be fitted to a 4 L (1 gal) bottle of working calcium chloride solution placed on a shelf $915 \pm 25\text{ mm}$ ($36 \pm 1\text{ in.}$) above the work surface.
- Measuring can: With a capacity of $85 \pm 5\text{ mL}$ (3 oz.).
- Funnel: With a wide-mouth for transferring sample into the graduated cylinder.
- Quartering cloth: 600 mm (2 ft) square nonabsorbent cloth, such as plastic or oilcloth.
- Mechanical splitter: See the FOP for AASHTO T 248.
- Strike-off bar: A straightedge or spatula.
- Clock or watch reading in minutes and seconds.
- Manually-operated sand equivalent shaker: Capable of producing an oscillating motion at a rate of 100 complete cycles in $45 \pm 5\text{ seconds}$, with a hand assisted half stroke length of $127 \pm 5\text{ mm}$ ($5 \pm 0.2\text{ in.}$). It may be held stable by hand during the shaking operation. It is recommended that this shaker be fastened securely to a firm and level mount, by bolts or clamps, if a large number of determinations are to be made.
- Mechanical shaker: See AASHTO T 176 for equipment and procedure.
- Oven: Capable of maintaining a temperature of $110 \pm 5^\circ\text{C}$ ($230 \pm 9^\circ\text{F}$).
- Thermometer: Calibrated liquid-in-glass or electronic digital type designed for total immersion and accurate to 0.1°C (0.2°F).

Materials

- Stock calcium chloride solution: Obtain commercially prepared calcium chloride stock solution meeting AASHTO requirements.
- Working calcium chloride solution: Dilute one 3 oz measuring can (85 ± 5 mL) of stock calcium chloride solution to 4 L (1 gal) with distilled or demineralized water. (The graduated cylinder filled to 111.8 mm [4.4 in.] contains 88 mL.)

Note 1: Mix the working solution thoroughly. Add 85 mL (3 oz.) of stock solution to a clean, empty 4 L (1 gal.) jug, add approximately 1 L (1 qt), and agitate vigorously for 2 or 3 minutes. Add the remainder of the water in approximately 1 L (1 qt) increments, repeating the agitation process.

Note 2: Tap water may be used if it is proven not to be detrimental to the test and if it is allowed by the agency.

Note 3: The shelf life of the working solution is approximately 30 days. Working solutions more than 30 days old shall be discarded.

Temperature Control

The temperature of the working solution should be maintained at $22 \pm 3^{\circ}\text{C}$ ($72 \pm 5^{\circ}\text{F}$) during the performance of the test. If field conditions preclude the maintenance of the temperature range, reference samples should be submitted to the Central/Regional Laboratory, as required by the agency, where proper temperature control is possible. Samples that meet the minimum sand equivalent requirement at a working solution temperature outside of the temperature range need not be subject to reference testing.

Sample Preparation

1. Obtain the sample in accordance with the FOP for AASHTO T 2 and reduce in accordance with the FOP for AASHTO T 248.
2. Prepare sand equivalent test samples from the material passing the 4.75 mm (No. 4) sieve. If the material is in clods, break it up and re-screen it over a 4.75 mm (No. 4) sieve. All fines shall be cleaned from particles retained on the 4.75 mm (No. 4) sieve and included with the material passing that sieve.
3. Split or quarter 1000 to 1500 g of material from the portion passing the 4.75 mm (No. 4) sieve. Use extreme care to obtain a truly representative portion of the original sample.

Note 4: Experiments show that, as the amount of material being reduced by splitting or quartering is decreased, the accuracy of providing representative portions is reduced. It is imperative that the sample be split or quartered carefully. When it appears necessary, dampen the material before splitting or quartering to avoid segregation or loss of fines.

Note 5: All tests, including reference tests, will be performed utilizing Alternative Method No. 2 as described in AASHTO T 176, unless otherwise specified.

4. The sample must have the proper moisture content to achieve reliable results. This condition is determined by tightly squeezing a small portion of the thoroughly mixed sample in the palm of the hand. If the cast that is formed permits careful handling without breaking, the correct moisture content has been obtained.

Note 6: Clean sands having little 75 μm (No. 200), such as sand for Portland Cement Concrete (PCC), may not form a cast.

If the material is too dry, the cast will crumble and it will be necessary to add water and remix and retest until the material forms a cast. When the moisture content is altered to provide the required cast, the altered sample should be placed in a pan, covered with a lid or with a damp cloth that does not touch the material, and allowed to stand for a minimum of 15 minutes. Samples that have been sieved without being air-dried and still retain enough natural moisture are exempted from this requirement.

If the material shows any free water, it is too wet to test and must be drained and air dried. Mix frequently to ensure uniformity. This drying process should continue until squeezing provides the required cast.

5. Place the sample on the quartering cloth and mix by alternately lifting each corner of the cloth and pulling it over the sample toward the diagonally opposite corner, being careful to keep the top of the cloth parallel to the bottom, thus causing the material to be rolled. When the material appears homogeneous, finish the mixing with the sample in a pile near the center of the cloth.
6. Fill the measuring can by pushing it through the base of the pile while exerting pressure with the hand against the pile on the side opposite the measuring can. As the can is moved through the pile, hold enough pressure with the hand to cause the material to fill the tin to overflowing. Press firmly with the palm of the hand, compacting the material and placing the maximum amount in the can. Strike off the can level full with the straightedge or spatula.
7. When required, repeat steps 5 and 6 to obtain additional samples.

Procedure

1. Start the siphon by forcing air into the top of the solution bottle through the tube while the pinch clamp is open.
2. Siphon 101.6 \pm 2.5 mm (4 \pm 0.1 in.) of working calcium chloride solution into the plastic cylinder. Pour the prepared test sample from the measuring can into the plastic cylinder, using the funnel to avoid spilling. Tap the bottom of the cylinder sharply on the heel of the hand several times to release air bubbles and to promote thorough wetting of the sample.
3. Allow the wetted sample to stand undisturbed for 10 \pm 1 minutes. At the end of the 10-minute period, stopper the cylinder and loosen the material from the bottom by simultaneously partially inverting and shaking the cylinder.
4. After loosening the material from the bottom of the cylinder, shake the cylinder and contents by any one of the following methods:
 - a. Mechanical Method – Place the stoppered cylinder in the mechanical shaker, set the timer, and allow the machine to shake the cylinder and contents for 45 \pm 1 seconds.

Caution: Agencies may require additional operator qualifications for the next two methods.

- b. Manually-operated Shaker Method – Secure the stoppered cylinder in the three spring clamps on the carriage of the manually-operated sand equivalent shaker and set the stroke counter to zero. Stand directly in front of the shaker and force the pointer to the stroke limit marker painted on the backboard by applying an abrupt horizontal thrust to the upper portion of the right hand spring strap.

Remove the hand from the strap and allow the spring action of the straps to move the carriage

and cylinder in the opposite direction without assistance or hindrance. Apply enough force to the right-hand spring steel strap during the thrust portion of each stroke to move the pointer to the stroke limit marker by pushing against the strap with the ends of the fingers to maintain a smooth oscillating motion. The center of the stroke limit marker is positioned to provide the proper stroke length and its width provides the maximum allowable limits of variation.

Proper shaking action is accomplished when the tip of the pointer reverses direction within the marker limits. Proper shaking action can best be maintained by using only the forearm and wrist action to propel the shaker. Continue shaking for 100 strokes.

- c. Hand Method – Hold the cylinder in a horizontal position and shake it vigorously in a horizontal linear motion from end to end. Shake the cylinder 90 cycles in approximately 30 seconds using a throw of $229 \text{ mm} \pm 25 \text{ mm}$ ($9 \pm 1 \text{ in.}$). A cycle is defined as a complete back and forth motion. To properly shake the cylinder at this speed, it will be necessary for the operator to shake with the forearms only, relaxing the body and shoulders.
5. Set the cylinder upright on the work table and remove the stopper.
 6. Insert the irrigator tube in the cylinder and rinse material from the cylinder walls as the irrigator is lowered. Force the irrigator through the material to the bottom of the cylinder by applying a gentle stabbing and twisting action while the working solution flows from the irrigator tip. Work the irrigator tube to the bottom of the cylinder as quickly as possible, since it becomes more difficult to do this as the washing proceeds. This flushes the fine material into suspension above the coarser sand particles.

Continue to apply a stabbing and twisting action while flushing the fines upward until the cylinder is filled to the 381 mm (15 in.) mark. Then raise the irrigator slowly without shutting off the flow so that the liquid level is maintained at about 381 mm (15 in.) while the irrigator is being withdrawn. Regulate the flow just before the irrigator is entirely withdrawn and adjust the final level to 381 mm (15 in.).

Note 7: Occasionally the holes in the tip of the irrigator tube may become clogged by a particle of sand. If the obstruction cannot be freed by any other method, use a pin or other sharp object to force it out, using extreme care not to enlarge the size of the opening. Also, keep the tip sharp as an aid to penetrating the sample.

7. Allow the cylinder and contents to stand undisturbed for 20 minutes ± 15 seconds. Start timing immediately after withdrawing the irrigator tube.

Note 8: Any vibration or movement of the cylinder during this time will interfere with the normal settling rate of the suspended clay and will cause an erroneous result.

8. Clay and sand readings:
 - a. At the end of the 20-minute sedimentation period, read and record the level of the top of the clay suspension. This is referred to as the clay reading.

Note 9: If no clear line of demarcation has formed at the end of the 20-minute sedimentation period, allow the sample to stand undisturbed until a clay reading can be obtained, then immediately read and record the level of the top of the clay suspension and the total sedimentation time. If the total sedimentation time exceeds 30 minutes, rerun the test using three individual samples of the same material. Read and record the clay column height of the sample requiring the shortest sedimentation period only. Once a sedimentation time has been established, subsequent tests will be run using that time. The time will be recorded along with the test results on all reports.

- b. After the clay reading has been taken, place the weighted foot assembly over the cylinder and gently lower the assembly until it comes to rest on the sand. Do not allow the indicator to hit the mouth of the cylinder as the assembly is being lowered. Subtract 254 mm (10 in.) from the level indicated by the extreme top edge of the indicator and record this value as the sand reading.

- c. If clay or sand readings fall between 2.5 mm (0.1 in.) graduations, record the level of the higher graduation as the reading. For example, a clay reading that appears to be 7.95 would be recorded as 8.0; a sand reading that appears to be 3.22 would be recorded as 3.3.
- d. If two Sand Equivalent (SE) samples are run on the same material and the second varies by more than ± 4 , based on the first cylinder result, additional tests shall be run.
- e. If three or more Sand Equivalent (SE) samples are run on the same material, average the results. If an individual result varies by more than ± 4 , based on the average result, additional tests shall be run.

Calculations

1. Calculate the SE to the nearest 0.1 using the following formula:

$$SE = \frac{\text{Sand Reading}}{\text{Clay Reading}} \times 100$$

2. Report the SE as the next higher whole number.
3. In determining the average of the two samples, raise each calculated SE value to the next higher whole number before averaging.

Report

Results shall be reported on standard forms approved for use by the agency.

Report results to the whole number.

This page intentionally left blank.

SPECIFIC GRAVITY AND ABSORPTION OF COARSE AGGREGATE WAQTC FOP FOR AASHTO T 85

Scope

This procedure covers the determination of specific gravity and absorption of coarse aggregate in accordance with AASHTO T 85. Specific gravity may be expressed as bulk specific gravity (G_{sb}), bulk specific gravity, saturated surface dry (G_{sb} SSD), or apparent specific gravity (G_{sa}). G_{sb} and absorption are based on aggregate after soaking in water. This procedure is not intended to be used with lightweight aggregates.

Terminology

Absorption – the increase in the mass of aggregate due to water being absorbed into the pores of the material, but not including water adhering to the outside surface of the particles, expressed as a percentage of the dry mass. The aggregate is considered “dry” when it has been maintained at a temperature of $110 \pm 5^{\circ}\text{C}$ ($230 \pm 9^{\circ}\text{F}$) for sufficient time to remove all uncombined water.

Saturated Surface Dry (SSD) – condition of an aggregate particle when the permeable voids are filled with water, but no water is present on exposed surfaces.

Specific Gravity – the ratio of the mass, in air, of a volume of a material to the mass of the same volume of gas-free distilled water at a stated temperature.

Apparent Specific Gravity (G_{sa}) – the ratio of the mass, in air, of a volume of the impermeable portion of aggregate to the mass of an equal volume of gas-free distilled water at a stated temperature.

Bulk Specific Gravity (G_{sb}) – the ratio of the mass, in air, of a volume of aggregate (including the permeable and impermeable voids in the particles, but not including the voids between particles) to the mass of an equal volume of gas-free distilled water at a stated temperature.

Bulk Specific Gravity (SSD) (G_{sb} SSD) – the ratio of the mass, in air, of a volume of aggregate, including the mass of water within the voids filled to the extent achieved by submerging in water for 15 to 19 hours (but not including the voids between particles), to the mass of an equal volume of gas-free distilled water at a stated temperature.

Apparatus

- Balance or scale: with a capacity of 5 kg, sensitive to 0.1 g. Meeting the requirements of AASHTO M 231.
- Sample container: a wire basket of 3.35 mm (No. 6) or smaller mesh, with a capacity of 4 to 7 L (1 to 2 gal) to contain aggregate with a nominal maximum size of 37.5 mm (1 1/2 in.) or smaller; and/or a larger basket for larger aggregates.
- Water tank: watertight and large enough to completely immerse aggregate and basket, equipped with an overflow valve to keep water level constant.
- Suspension apparatus: wire used to suspend apparatus shall be of the smallest practical diameter.
- Sieves 4.75 mm (No. 4) or other sizes as needed, conforming to AASHTO M 92.
- Large absorbent towel

Sample Preparation

1. Obtain the sample in accordance with the FOP for AASHTO T 2 (see Note 1).
2. Mix the sample thoroughly and reduce it to the approximate sample size required by Table 1 in accordance with the FOP for AASHTO T 248.
3. Reject all material passing the appropriate sieve by dry sieving.
4. Thoroughly wash sample to remove dust or other coatings from the surface and re-screen the washed dry sample over the appropriate sieve. Reject all material passing that sieve.
5. The sample shall meet or exceed the minimum mass given in Table 1.

Note 1: If this procedure is used only to determine the Bulk G_{sb} of oversized material for the FOP for AASHTO T 99 / T 180 and in the calculations for the FOP for AASHTO T 224, the material can be rejected over the appropriate sieve. For T 99 / T 180 Methods A & B, use the 4.75 mm (No.4) sieve; T 99 / T 180 Methods C & D use the 19 mm (3/4 in).

Table 1

Nominal Maximum Size mm (in.)	Minimum Mass of Test Sample, g (lb)
12.5 (1/2) or less	2,000 (4.4)
19.0 (3/4)	3,000 (6.6)
25.0 (1)	4,000 (8.8)
37.5 (1-1/2)	5,000 (11)
50 (2)	8,000 (18)
63 (2-1/2)	12,000 (26)
75 (3)	18,000 (40)

* One sieve larger than the first sieve to retain more than 10 percent of the material using an agency specified set of sieves based on cumulative percent retained. Where large gaps in specification sieves exist, intermediate sieve(s) may be inserted to determine nominal maximum size.

Procedure

1. Dry the test sample to constant mass at a temperature of $110 \pm 5^{\circ}\text{C}$ ($230 \pm 9^{\circ}\text{F}$) and cool in air at room temperature for 1 to 3 hours.

Note 2: Where the absorption and specific gravity values are to be used in proportioning concrete mixtures in which the aggregates will be in their naturally moist condition, the requirement for initial drying to constant mass may be eliminated, and, if the surfaces of the particles in the sample have been kept continuously wet until test, the 15-to-19 hour soaking may also be eliminated.

2. Immerse the aggregate in water at room temperature for a period of 15 to 19 hours.

Note 3: When testing coarse aggregate of large nominal maximum size requiring large test samples, it may be more convenient to perform the test on two or more subsamples, and then combine the values obtained.

3. Place the empty basket into the water bath and attach to the balance. Inspect the immersion tank to ensure the water level is at the overflow outlet height. Tare the balance with the empty basket attached in the water bath.
4. Remove the test sample from the water and roll it in a large absorbent cloth until all visible films of water are removed. Wipe the larger particles individually.

Note 4: A moving stream of air may be used to assist in the drying operation, but take care to avoid evaporation of water from aggregate pores.

5. Determine the SSD mass of the sample, and record this and all subsequent masses to the nearest 0.1 g or 0.1 percent of the sample mass, whichever is greater. Designate this mass as “B”.
6. Re-inspect the immersion tank to insure the water level is at the overflow outlet height. Immediately place the SSD test sample in the sample container and weigh it in water maintained at $23.0 \pm 1.7^{\circ}\text{C}$ ($73.4 \pm 3^{\circ}\text{F}$). Shake the container to release entrapped air before recording the weight. Designate this submerged weight as “C”.

Note 5: The container should be immersed to a depth sufficient to cover it and the test sample during mass determination. Wire suspending the container should be of the smallest practical size to minimize any possible effects of a variable immersed length.

7. Remove the sample from the basket. Ensure all material has been removed. Place in a container of known mass.
8. Dry the test sample to constant mass in accordance with the FOP for AASHTO T 255 / T 265 (Aggregate section) and cool in air at room temperature for 1 to 3 hours. Designate this mass as “A”.

Calculations

Perform calculations and determine values using the appropriate formula below. In these formulas, A = oven dry mass, B = SSD mass, and C = weight in water.

Bulk specific gravity (G_{sb})

$$G_{sb} = A / (B - C)$$

Bulk specific gravity, SSD (G_{sb} SSD)

$$G_{sb} \text{ SSD} = B / (B - C)$$

Apparent specific gravity (G_{sa})

$$G_{sa} = A / (A - C)$$

Absorption

$$\text{Absorption} = [(B - A) / A] \times 100$$

Report

Results shall be reported on standard forms approved by the agency. Report specific gravity values to 3 decimal places and absorption to 0.1 percent.

Addendum WAQTC FOP for AASHTO T 85

Following are guidelines for the use of WAQTC FOP for AASHTO T 85 by the State of Alaska DOT&PF.

1. When Specific Gravity is determined on portions of the sample, determine to total sample specific gravity with the following formula:

$$G = \frac{1}{\frac{P_1}{100 \times G_1} + \frac{P_2}{100 \times G_2} + \dots + \frac{P_n}{100 \times G_n}}$$

Where:

G= average specific gravity

P₁, P₂, P_n, = mass percentages of each portion tested from the original sample;

G₁, G₂, G_n, = specific gravity values of each portion tested from the original sample;

Relative Standard Density of Soils by the Control Strip Method

ATM 309

1. Scope

This method describes a procedure for determining the relative standard density of a material by the control strip testing method. This is applicable to soils and soil mixtures.

2. Significance and Use

Site conditions and/or logistics may make determining the standard density difficult with conventional test methods used in the laboratory. When these problems occur a method that allows the determination of a relative standard density in the field can facilitate the verification of compaction efforts. This method describes a procedure to determine the relative standard density to be used in these circumstances.

3. Apparatus

- Nuclear Moisture/Density Gauge—Calibrate and standardize in accordance with WAQTC FOP for AATSHOTO T 310.
- Compaction equipment that meets the requirements of the contract and of sufficient size and compaction energy to compact the material.

4. Site Preparation

1. The Engineer will designate the location and the size of the control strip, as well as minimum compaction equipment to be used.
2. A representative lift of the material being evaluated will be placed and prepared for compaction.

5. Procedure

1. Attention should be paid to the requirements of the material being placed so that moisture requirements are maintained in an acceptable range.
2. A minimum of 3 test locations will be selected with-in the control strip. The locations will be in the middle 1/2 of the control strip and at least 12 in from the edge of the control strip. The Engineer will select test locations.
3. The locations will be marked in such a way as not to be lost during the compaction of the control strip. This can be accomplished by marking the side of the strip with stakes or surveyors tape, or by marking with paint beside the location on the control strip.
4. Tests shall be taken in backscatter mode. A test will consist of a 15 second (fast mode), or 1 minute, or the average of two dry density determination at each location as approved by the engineer.
5. Care should be taken when preparing the test location so that it is flat and the surface voids filled. If necessary, use a small quantity of fines to fill the voids. This layer will in no case be more than 1/8 in depth.

6. After the first pass with the compaction equipment, an initial density test is taken and recorded.

Note 1: One pass of the roller will be defined as one roll over the location.

7. After each subsequent pass and for each piece of compaction equipment used, a test is taken at each location and recorded.
8. Continue the compaction and testing cycle until either of these conditions is met:

- a. There is less than 1 lb/ft³ increase in the dry density of the average density tests for each location on two consecutive passes.
 - b. There is less than 1 lb/ft³ increase in the dry density of the average of all three locations for two consecutive passes.
9. Select ten random locations on the completed control strip and test by averaging two one minute counts at each location in accordance with WAQTC FOP for AASHTO T 310. Average the results from the ten locations and this value will be the relative standard density for this material. Tests shall be done with direct transmission when practicable.
- Note 2: It may be necessary to repeat the procedure for additional roller types depending on the material to be tested and the requirements of sequencing for the finished surface.
10. Additional control strips may be required if there are changes in the material, lift thickness or compaction equipment.

6. Calculations

1. The Relative Standard Density value will be calculated as follows:

$$D_s = \frac{(A_1 + A_2 + A_3 + A_4 + A_5 + A_6 + A_7 + A_8 + A_9 + A_{10})}{10}$$

Where:

D_s = Relative Standard Density for the material.

A_n = Average Density for random test location n .

7. Report

- Report the average density for each pass
- Report the standard density to the nearest 0.1 lb/ft³

Nordic Abrasion Value of Coarse Aggregate ATM 312

1. Scope

This method describes the test procedure for the simulation of the abrasive action of traffic on coarse aggregates used in a surface layer to determine the ability of the aggregate to resist wear by abrasion from studded tires.

The test shall be performed on aggregates with a size fraction of 11.2 to 16.0 mm (7/16" to 5/8")

Note 1: Variations from this size range will not give consistent results.

The test is applicable to crushed and uncrushed natural and artificial aggregates.


This test method involves potentially hazardous materials, operations and equipment. This method does not purport to address all of the safety problems associated with its use.

2. Principle

A sample of a single-sized aggregate group, 11.2 to 16.0 mm (7/16" to 5/8"), is rotated together with steel balls and water in a steel drum. Three ribs, which are mounted on the interior of the drum, add to the abrading action of the aggregate particles and the steel balls. The contents roll within the drum with an abrading action. After the specified number of revolutions, the contents are removed from the drum and the aggregate portion is sieved on a 2.00 mm (No. 10) sieve to measure the wear as a percentage loss.

3. Apparatus

- Testing machine conforming to the design shown in Figure 1.
- The cylinder shall have an inside diameter of 206.5 ± 2 mm and an inside length of 335 ± 1 mm. Three ribs, each with a length of 333 ± 1 mm, shall be equally spaced around the internal circumference of the cylinder. The test drum shall be water-tight and made of a seamless steel tube conforming to grade *TS 5 of ISO 2604-2*, of outside diameter 219.1 mm and wall thickness of 6.3 mm. The cylinder shall rotate centrically with the axis in a horizontal position at a rate of 90 ± 3 rpm. A revolution counter shall automatically stop the rotation after 5400 revolutions.
- The three ribs shall be removable and made from spring steel as specified in *ISO 683-14* and designed in accordance with figure 1. The ribs, prior to their use in the test, shall be preground in the drum for 25 h using a hard aggregate, together with the normal proportions of steel balls and water.
- During the test the ribs will wear and their action will change. Each rib shall be replaced, when its loss in original mass exceeds 15 g.
- Ball bearings, 14.99-15.05 mm diameter, of a hardness between 62 and 65 HRC, as specified in *ISO*

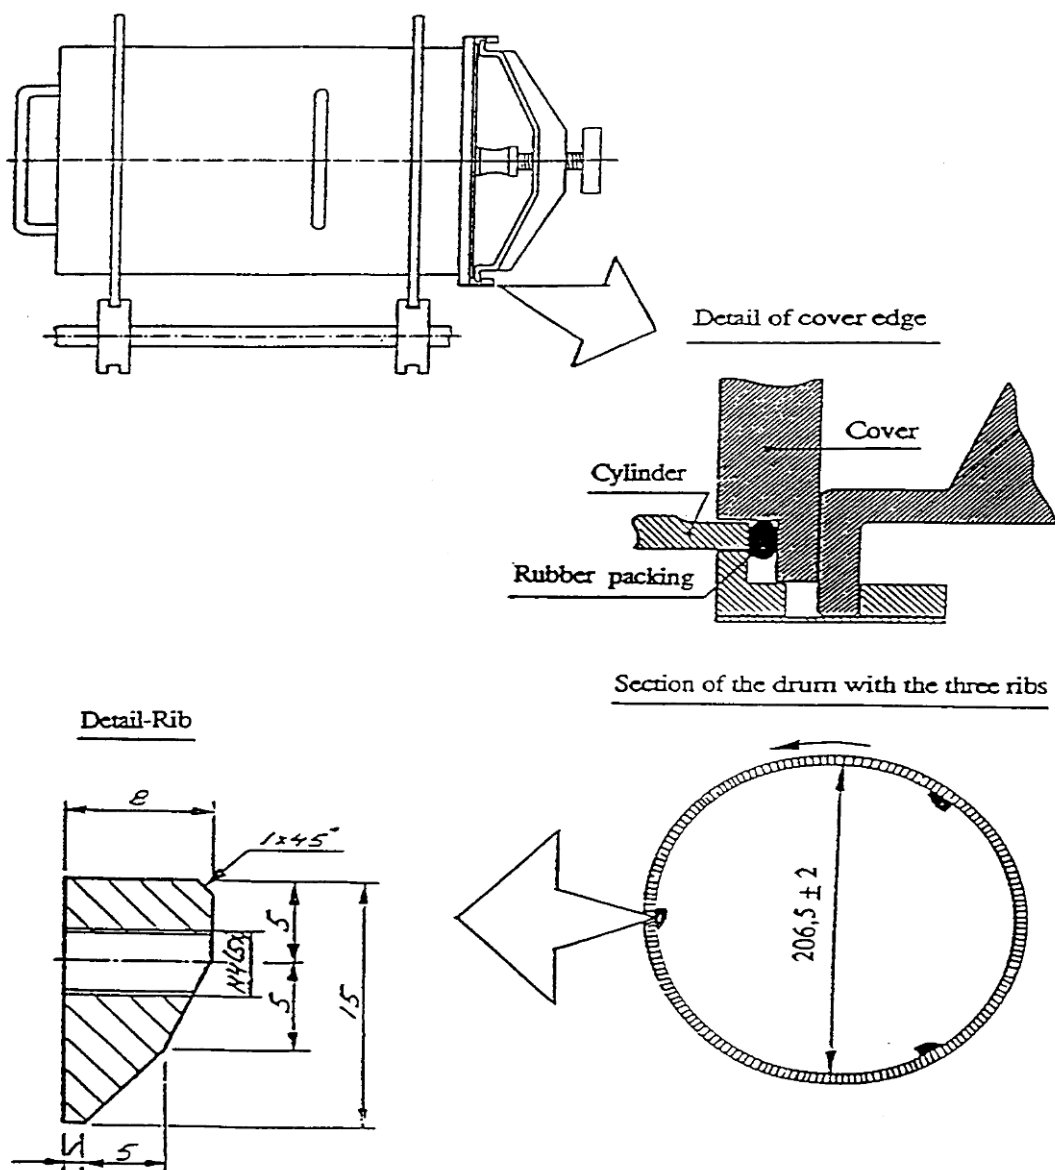

3290.

Figure 1

- Gauge to control minimum ball size, e.g. two parallel bars 14.5 mm apart.
- Magnet (optional) for removal of the charge from the aggregate test sample after abrasion.

Note 3: Do not use too strong a magnet as the balls may become magnetized.

- Oven capable of maintaining a uniform temperature of $110 \pm 5^{\circ}\text{C}$ ($230 \pm 9^{\circ}\text{F}$).
- Balance or scale: Capacity sufficient for the principle sample mass, readable to 0.1 percent or 0.1 g, of the total sample mass and meeting the requirements of AASHTO M 231.
- Sieves of the following sizes: 2.00 mm, 11.2 mm, and 16.0 mm (No. 10, 7/16" and 5/8").
- Bucket.
- Washing device.

4. Sampling

Obtain the sample in accordance with WAQTC FOP for AASHTO T 2.

5. Preparation Of Test Sample

Unprocessed Aggregate

1. Separate the sample on the 19 mm (3/4") sieve by hand or mechanical shaker, sieving the material for 5 minutes. Discard the minus 19 mm (3/4") material unless required for other testing.
2. Crush the plus 19 mm (3/4") aggregate, or a representative portion obtained in accordance with WAQTC FOP for AASHTO T 248, to pass the 19 mm (3/4") sieve. 3. Separate the material into the required test size, using 16 mm (5/8") sieve and 11.2 mm (7/16") sieves, in accordance with WAQTC FOP for AASHTO T 27/T 11. Discard all particles retained on the 16 mm (5/8") sieve and all the particles passing the 11.2 mm (7/16") sieve, unless required for other testing.
4. Proceed to Step 2 below.

Processed (already crushed) Aggregate

1. Separate the material into the required test size, using 16 mm (5/8") and 11.2 mm (7/16") sieves, in accordance with WAQTC FOP for AASHTO T 27/T 11. Discard all particles retained on the 5/8" (16 mm) sieve and all the particles passing the 11.2 mm (7/16") sieve, unless required for other testing.
2. Sample must have no more than 8 percent Flat and Elongated when tested in accordance with ATM 306 using a caliper ratio of 1:5.
3. Reduce the sample to test size (minimum of 3500 g) in accordance with WAQTC FOP for AASHTO T 248.
4. Wash the sample and dry to a constant mass in accordance with WAQTC FOP for AASHTO T 255/T 265.
5. Determine the apparent specific gravity of the sample, or a portion thereof, in accordance with WAQTC FOP for AASHTO T 85.
6. Determine the test sample mass by:

$$m_i = \frac{P_i}{2.66} \times 1000$$

Where m_i = mass of the test sample

p_i = apparent specific gravity of test sample.

7. Batch 3 test specimens at the calculated weight ± 5 g.

6. Procedure

1. Place the ball charge (7000 ± 10 g) and the test sample in the drum and add (2000 ± 10) ml. of water.
2. Rotate the drum at a speed of 90 ± 3 rpm for 5400 ± 10 revolutions.
3. After the specified number of revolutions, discharge the contents (sample and ball charge) from the drum into a bucket.
4. Wash the sample including the ball charge on a 2.00 mm (No. 10) sieve. Remove the steel balls from the sample with a magnet.

Note 4: To avoid overloading the sieve, it may be necessary to divide the sample into smaller portions.

5. Dry the aggregate fraction retained on the 2.00 mm (No. 10) sieve, to a constant mass in accordance with WAQTC FOP for AASHTO T 255 and weigh to the nearest 0.1 g.

7. Calculation and Expression of Results

1. Calculate the individual Nordic Abrasion Values (A_N) to the nearest 0.1 percent as follows:

$$A_N = \left(\frac{M_i - M_f}{M_i} \right) \times 100$$

Where M_i = Initial dry mass of the test sample.

M_f = Dry mass of the aggregate after the test.

2. Compute and record the average of the individual Nordic Abrasion Values to the nearest 0.1 percent.

8. Report

The individual and average Nordic Abrasion values shall be reported on Department forms to the nearest 0.1 percent.

Degradation Value of Aggregates ATM 313

1. Scope

This test method describes the procedure for determining the durability of an aggregate. The durability of an aggregate as measured by the Degradation Value indicates the relative resistance of an aggregate to produce detrimental clay-like fines when subjected to a prescribed abrasion process in the presence of distilled or demineralized water.

2. Apparatus

- Jaw crusher with 150 mm (6") capacity.
- Sieves of the following sizes: 12.5 mm (½"), 6.3 mm (¼"), 2.00 mm (No. 10) and 75 µm (No. 200). Sieves shall conform to AASHTO M 92.
- Balance or scale: Capacity sufficient for the principle sample mass, readable to 0.1 percent or 0.1 g of the total sample mass and meeting the requirements of AASHTO M 231.
- 200 mm (8") sieve shaker with 45 mm (1¾") throw on cam at 285 ± 10 oscillations per minute.
- General Laboratory Interval Timer to control On-Off operation of sieve shaker. Timer will have a minimum 20 minute range accurate to ± 5 seconds.
- Plastic canister 190 mm (7½") in diameter and 150 mm (6") high, having a flat bottom or metal washing vessel conforming to AASHTO T 210 - 5.1.
- Distilled or demineralized water maintained at $22 \pm 3^{\circ}\text{C}$ ($72 \pm 5^{\circ}\text{F}$).
- Sample Washing Apparatus, consisting of a ring stand and ring capable of mounting a 230 mm mouth funnel with a 2.00 mm (No. 10) and 75 µm (No. 200) sieve setting on top of the funnel and a graduated cylinder calibrated at 500 ml with a rubber stopper.
- Graduated cylinder or pipette with 10 ml capacity graduated in 1 ml increments.
- Stock Sand Equivalent Solution prepared in accordance with WAQTC FOP for AASHTO T 176, using distilled water only. This solution should be stored in dark or opaque containers and protected from direct sunlight and heat. Solutions that have turned cloudy or formed precipitates will be discarded.
- Standard Sand Equivalent Cylinder with rubber stopper as described in WAQTC FOP for AASHTO T 176.
- Timer or Stopwatch, preferably with an alarm to indicate end of timed interval.
- Miscellaneous equipment including 500 ml wash bottle with a fine spray nozzle, pans, scoops, etc.

3. Degradation Test Area

The degradation test area must be free of vibration and direct sunlight, and maintained at a temperature of $22 \pm 3^{\circ}\text{C}$ ($72 \pm 5^{\circ}\text{F}$).

4. Sample Preparation

1. Unprocessed Aggregate

- a. Separate the aggregate on the 12.5 mm (½") sieve by hand or by mechanical shaker, sieving the material for 5 minutes. Discard the minus 12.5 mm (½") material unless required for other testing.
- b. Crush the plus 12.5 mm (½") aggregate, or a representative portion obtained in accordance with WAQTC

FOP for AASHTO T 248, to pass the 12.5 mm (½") sieve.

c. Proceed to Step 2 and process the same as already crushed aggregate.

2. Processed (already crushed) Aggregate

- a. Separate the material by hand sieving or by mechanical shaker, sieving the material for 5 minutes, into 2 size groups: minus 12.5 mm (½") to plus 6.3 mm (¼") and minus 6.3 mm (¼") to plus 2.00 mm (No. 10).
- b. Reduce each size grouping to a representative sample in accordance with WAQTC FOP for AASHTO T 248, Method A, such that there will be a minimum of 500 grams after washing.
- c. Wash each size grouping over a 2.00 mm (No. 10) sieve and dry to a constant mass in accordance with WAQTC FOP for AASHTO T 255/T 265.
- d. Weigh out a 500 ±1 g portion of each size grouping.

5. Procedure

1. Combine both sample portions in the plastic canister, add 200 ml of distilled or demineralized water and cover tightly. Do not allow the sample to soak more than 5 minutes before testing.
2. Place the canister in the degradation sieve shaker and run for 20 minutes ±5 seconds. Do not allow the sample to set for more than 5 minutes after agitation is completed.
3. Remove the canister and wash the material through nested 2.00 mm (No. 10) and 75 µm (No. 200) sieves. Continue washing until the wash water is clear and has reached the 500-ml mark on the graduated cylinder.
4. In instances where highly degradable materials are encountered and the sample cannot be washed clean with 500-ml. of water:
 - a. Continue washing using water sparingly, until the wash water is clear. If a change in receiver cylinders is required, be very careful not to lose any of the wash water.
 - b. To achieve the required 500 ml. volume, allow the wash water to settle until clear, then siphon or pipette off the excess water, being careful not to remove any of the settled material.
 - c. Use of a centrifuge to settle the material is allowed but extreme care must be taken to preclude any loss of material in transferring from the cylinders to the centrifuge bottles and then back to a single cylinder. The solution must be brought to a volume of 500 ml before proceeding to Step 5. Removal of extra water by oven-dried evaporation is not allowed.
5. Place the Sand Equivalent Cylinder upright in a vibration free area out of direct sunlight. Measure and pour 7 ml of the Stock Sand Equivalent Solution into the cylinder.
6. Bring all of the solids in the 500 ml of wash water into suspension by capping the graduated cylinder with the palm of the hand or a rubber stopper, then turning the graduated cylinder upside down and right side up 10 times or until material is in suspension, allowing the bubble to traverse from one end to the other and back again, as rapidly as possible (approximately 35 seconds).
7. Immediately pour the solution into the Sand Equivalent Cylinder, fill to the 15 mark, and plug with a rubber stopper.
8. Mix the contents of the Sand Equivalent Cylinder by turning the cylinder upside down and right side up allowing the bubble to traverse from one end to the other and back again. This is one cycle. Repeat this cycle 20 times as rapidly as possible (approximately 35 seconds).
9. Place the cylinder on a vibration free platform out of direct sunlight, remove stopper and immediately start the

timer or stopwatch that is pre-set for 20 minutes.

10. After 20 minutes, immediately read and record the height of the sediment to the nearest 0.1 graduation.

6. Calculations

Determine the Degradation Value by Table I, next page, which is derived from the following formula.

$$D = \left(\frac{15 - H}{15 + 1.75H} \right) \times 100$$

Where:

D = Degradation value.

H = Height of sediment in cylinder.

Values may range from 0 to 100 with high values representing more suitable material. The formula and chart place doubtful materials at about the midrange (30-70) of the scale, with poor ones below and good ones above that range.

7. Report

Report degradation values to the nearest whole number.

Table 1
Degradation Value, "D"

<u>H</u>	<u>D</u>		<u>H</u>	<u>D</u>		<u>H</u>	<u>D</u>		<u>H</u>	<u>D</u>		<u>H</u>	<u>D</u>
0.1	98		3.1	58		6.1	35		9.1	19		12.1	8
0.2	96		3.2	57		6.2	34		9.2	19		12.2	8
0.3	95		3.3	56		6.3	33		9.3	18		12.3	7
0.4	93		3.4	55		6.4	33		9.4	18		12.4	7
0.5	91		3.5	54		6.5	32		9.5	17		12.5	7
0.6	90		3.6	54		6.6	32		9.6	17		12.6	6
0.7	88		6.7	53		6.7	31		9.7	17		12.7	6
0.8	87		3.8	52		6.8	30		9.8	16		12.8	6
0.9	85		3.9	51		6.9	30		9.9	16		12.9	6
1.0	84		4.0	50		7	29		10.0	15		13.0	5
1.1	82		4.1	49		7.1	29		10.1	15		13.1	5
1.2	81		4.2	48		7.2	28		10.2	15		13.2	5
1.3	79		4.3	48		7.3	28		10.3	14		13.3	4
1.4	78		4.4	47		7.4	27		10.4	14		13.4	4
1.5	77		4.5	46		7.5	27		10.5	13		13.5	4
1.6	75		4.6	45		7.6	26		10.6	13		13.6	4
1.7	74		4.7	44		7.7	26		10.7	13		13.7	3
1.8	73		4.8	44		7.8	25		10.8	12		13.8	3
1.9	71		4.9	43		7.9	25		10.9	12		13.9	3
2.0	70		5.0	42		8	24		11.0	12		14.0	3
2.1	69		5.1	41		8.1	24		11.1	11		14.1	2
2.2	68		5.2	41		8.2	23		11.2	11		14.2	2
2.3	67		5.3	40		8.3	23		11.3	11		14.3	2
2.4	66		5.4	39		8.4	22		11.4	10		14.4	1
2.5	65		5.5	39		8.5	22		11.5	10		14.5	1
2.6	63		5.6	38		8.6	21		11.6	10		14.6	1
2.7	62		5.7	37		8.7	21		11.7	9		14.7	1
2.8	61		5.8	37		8.8	20		11.8	9		14.8	0
2.9	60		5.9	36		8.9	20		11.9	9		14.9	0
3.0	59		6.0	35		9.0	20		12.0	8		15.0	0

Expansive Breakdown of Stone on Soaking in Ethylene Glycol

ATM 314

1. Scope

This method covers a procedure for subjecting samples of stone to immersion in ethylene glycol and observation of the effects of such immersion in accordance with CRD-D 148-69.

2. Principle of Method

Ethylene glycol is one of the materials that reacts with swelling clays of the montmorillonite group to form an organo-clay complex having a larger basal spacing than that of the clay mineral itself. Hence a sample of stone containing swelling clay of the montmorillonite group will be expected to undergo expansive breakdown upon soaking in ethylene glycol, if the amount, distribution, state of expansion, and ability to take up glycol is such as to cause such breakdown to occur. If such breakdown does occur, it may be expected that similar breakdown may occur if similar rock samples are exposed, for longer times, to wetting and drying or freezing and thawing in a water soaked condition in service.

3. Reagent

Ethylene Glycol – The reagent used in this method shall be ethylene glycol meeting the requirements of ASTM D 2693.

4. Apparatus

- Jaw crusher with 150 mm (6 in) capacity.
- Sieves of the following sizes: 75 mm (3 in) and 19.0 mm ($\frac{3}{4}$ in) and conforming to AASHTO M 92.
- Balance or scale: Capacity sufficient for the principle sample mass, readable to 0.1 percent or 0.1 g of the total sample mass and meeting the requirements of AASHTO M 231.
- Container shall be of suitable plastic, non-reactive with the reagent and of sufficient size to hold the test sample and sufficient reagent to cover all particles of the sample to a depth of not less than 10 mm ($\frac{1}{2}$ in) capped with a tight-fitting cover.

5. Sampling and Sample Preparation

1. Obtain representative samples of the stone in accordance with WAQTC FOP for AASHTO T 2.
2. Crush the rock to pass a 75 mm (3 in) sieve.
3. Separate the material into the required test size, using 75 mm (3 in) and 19 mm ($\frac{3}{4}$ in) sieves, in accordance with WAQTC FOP for AASHTO T 27/T 11. Discard all particles retained on the 75 mm (3 in) sieve and all particles passing the 19 mm ($\frac{3}{4}$ in) sieve, unless required for other testing.
4. Reduce the sample to a test size of 5 ± 2 kg (11 ± 1 lb) in accordance with WAQTC FOP for AASHTO T 248, Method A.
5. When a sample of the required mass and particle size has been prepared, it shall be washed to remove dust, loosely adherent coatings, and chips. After being washed, dry to a constant mass in accordance with WAQTC FOP for AASHTO T 255/T 265 except that constant mass shall be regarded as having been attained when the loss in weight between successive weighing at intervals of not less than 4 hours does not exceed 0.1 percent. Determine the number of particles and the mass before immersion to the nearest 0.1 percent of the total sample mass.

6. Procedure

1. The sample shall be placed in the container and immersed in the reagent so that all particles are covered to a depth of at least 12.5 mm (½ in).
2. At intervals not to exceed 3 days, examine the sample and note significant changes. The normal duration of the test shall be 15 days.

Note 3: Further information of value may be obtained in certain cases by continuing the treatment beyond 15 days: in other cases expansive breakdown may have been too extensive at earlier periods that no information of value will be obtained by continuing the treatment for the full 15 days.

3. When the exposure has been terminated, the sample shall be thoroughly washed and sieved by hand over a 19 mm (¾ in) sieve to remove the reagent from the surfaces of the particles and to remove fragments that will pass a 19 mm (¾ in) sieve. The material remaining on the sieve shall be dried to constant weight as described in Step 4 of the Sampling and Sample Preparation, and the total mass after immersion determined to the nearest 0.1 percent of the total sample mass.

7. Calculations

Calculate the total percent loss by:

$$\left(\frac{M_B - M_A}{M_B} \right) \times 100$$

where:

M_B = Mass before immersion, and

M_A = Mass after immersion.

8. Report

Report the percent loss to the nearest 1 percent on department forms.

SAMPLING BITUMINOUS MATERIALS (See Addendum for DOT&PF Guidelines) **WAQTC FOP FOR AASHTO T 40**

Scope

The procedure covers obtaining samples of liquid bituminous materials in accordance with AASHTO T 40. Sampling of solid and semi-solid bituminous materials – included in AASHTO T 40 – is not covered here.

Agencies may be more specific on exactly who samples, where to sample, and what type of sampling device to use.

Warning: Always use appropriate safety equipment and precautions for hot liquids.

Procedure

1. Coordinate sampling with contractor or supplier.
2. Allow a minimum of 4 L (1 gal) to flow before obtaining a sample(s).
3. Obtain samples of:
 - Asphalt binder from hot mix asphalt (HMA) plant from the line between the storage tank and the mixing plant while the plant is in operation, or from the delivery truck.
 - Cutback and emulsified asphalt from distributor spray bar or application device; or from the delivery truck before it is pumped into the distributor. Sample emulsified asphalt at delivery or prior to dilution.

Containers

Sample containers must be new, and the inside may not be washed or rinsed. The outside may be wiped with a clean, dry cloth.

All samples shall be put in 1 L (1 qt) containers and properly identified on the outside of the container with contract number, date sampled, data sheet number, brand and grade of material, and sample number. Include lot and subplot numbers when appropriate.

- Emulsified asphalt: Use wide-mouth plastic jars with screw caps. Protect the samples from freezing since water is a part of the emulsion. The sample container should be completely filled to minimize a skin formation on the sample.
- Asphalt binder and cutbacks: Use metal cans.

Note: The sample container shall not be submerged in solvent, nor shall it be wiped with a solvent saturated cloth. If cleaning is necessary, use a clean dry cloth.

Addendum WAQTC FOP for AASHTO T 40

The following guidelines for the use of WAQTC FOP for AASHTO T 40 by the State of Alaska DOT&PF.

1. When obtaining samples from HMA plants, sample only from the line between the storage tank and the mixing plant while the plant is in operation.
2. Sample containers for elastomer modified asphaltic cements shall conform to requirements under containers/asphalt binders.
3. When sampling emulsified asphalt, use 1 gallon wide mouth plastic containers.
4. When material is sampled by other than DOT&PF personnel or their agent(s), the sampling must be witnessed and possession of the sample transferred immediately to DOT&PF personnel or their agent(s).

SAMPLING OF BITUMINOUS PAVING MIXTURES

FOP FOR AASHTO T 168 (See Addendum for DOT&PF Guidelines)

Scope

This procedure covers the sampling of bituminous paving mixtures from HMA plants, haul units, and roadways in accordance with AASHTO T 168. Sampling is as important as testing, and every precaution must be taken to obtain a truly representative sample.

Apparatus

- Shovel
- Sample containers: such as cardboard boxes, metal cans, stainless steel bowls, or other agency-approved containers
- Scoops, trowels, or other equipment to obtain mix
- Sampling plate: heavy gauge metal plate 380 mm x 380 mm (15 in x 15 in) minimum 8 gauge thick, with a wire attached to one corner long enough to reach from the center of the paver to the outside of the farthest auger extension. Holes ¼" in diameter should be provided in each corner.
- Cookie cutter sampling device: A 330 mm (13 in.) square sampling template, constructed from 75 mm x 50 mm x 3 mm (3 in. x 2 in. x 1/8 in.) formed steel angle with two 100mm x 150 mm x 9 mm (4 in. x 6 in. x 3/8 in.) handles. See diagram.

Note 1: Sampling Plate and Cookie cutter may be sized appropriately to accommodate sample size requirements.

- Mechanical sampling device

Sample Size

Sample size depends on the test methods specified by the agency for acceptance. Check agency requirement for the size required.

Sampling

General

1. The material shall be tested to determine variations. The supplier/contractor shall provide equipment for safe and appropriate sampling, including sampling devices on plants when required.
2. Place dense graded mixture samples in cardboard boxes, stainless steel bowls or other agency-approved containers. Place open graded mixture samples in stainless steel bowls. Do not put open graded mixture samples in boxes until they have cooled to the point that bituminous material will not migrate from the aggregate.

Attached Sampling Devices

Some agencies require mechanical sampling devices for hot mix asphalt (HMA) and cold feed aggregate on some projects. These are normally permanently attached devices that allow a sample container to pass perpendicularly through the entire stream of material or divert the entire stream of material into the container. Operation may be hydraulic, pneumatic, or manual and allows the sample container to pass through the stream twice, once in each direction, without overfilling. Special caution is necessary with manually operated systems since a consistent speed is difficult to maintain and non-representative samples may result. Check agency requirements for the specifics of required sampling systems.

1. Lightly coat the container attached to the sampling device with an agency-approved release agent and/or preheat it to approximately the same discharge temperature of the mix.
2. Pass the container twice through the material perpendicularly without overfilling the container.
3. Repeat until proper sample size has been obtained.
4. Transfer the HMA to an agency-approved container without loss of material.

Sampling from Haul Units

1. Visually divide the haul unit into approximately four equal quadrants.
2. Identify one sampling location in each quadrant.
3. Dig down and remove approximately 0.3 m (1 ft) of material to avoid surface segregation. Obtain each increment from below this level.
4. Combine the increments to form a sample of the required size.

Sampling from Roadway Prior to Compaction (Plate Method)

Plate method using the “cookie cutter” sampling device.

There are two conditions that will be encountered when sampling hot mix asphalt (HMA) from the roadway prior to compaction. The two conditions are:

1. Laying HMA on grade or untreated base material requires Method 1.
2. Laying HMA on existing asphalt or laying a second lift of HMA requires Method 2.

SAFETY:

Sampling is performed behind the paving machine and in front of the breakdown roller. For safety, the roller must remain at least 3 m (10 ft) behind the sampling operation until the sample has been taken and the hole filled with loose HMA.

Method 1 requires a plate to be placed in the roadway in front of the paving operation and therefore there is always concern with moving, operating equipment. It is safest to stop the paving train while a plate is installed in front of the paver. When this is not possible the following safety rules must be followed.

1. The plate placing operation must be at least 3 m (10 ft) in front of the paver or pickup device. The technician placing the plate must have eye contact and communication with the paving machine operator. If eye contact cannot be maintained at all time, a third person must be present to provide communication between the operator and the technician.
2. No technician is to be between the asphalt supply trucks and the paving machine. The exception to this rule is if the supply truck is moving forward creating a windrow, in which case the technician must be at least 3m (10 ft) behind the truck.

If at any time the Engineer feels that the sampling technique is creating an unsafe condition, the operation is to be halted until it is made safe or the paving operation will be stopped while the plate is being placed.

Method 1 - Obtaining a Sample on Untreated Base:

1. Following the safety rules detailed above, the technician is to:
 - a. Smooth out a location in front of the paver at least 0.5 m (2 ft) inside the edge of the mat.
 - b. Lay the plate down diagonally with the direction of travel, keeping it flat and tight to the base with the lead corner facing the paving machine.
2. Secure the plate in place by driving a nail through the hole in the lead corner of the plate.
3. Pull the wire, attached to the outside corner of the plate, taut past the edge of the HMA mat and secure with a nail.
4. Let the paving operation proceed over the plate and wire. Immediately proceed with the sampling.
5. Using the exposed end of the wire, pull the wire up through the fresh HMA to locate the corner of the plate. Place the “cookie cutter” sample device, just inside the end of the wire; align the cutter over the plate. Press “cookie cutter” device down through the HMA to the plate.
6. Using a small square tipped shovel and/or scoop, carefully remove all the HMA from inside of the cutter and place in a sample container. Care shall be taken to prevent contamination of bituminous mixes by dust or other foreign matter, and to avoid segregation of aggregate and bituminous materials.
7. Remove the sample cutter and the plate from the roadway. The hole made from the sampling must be filled by the contractor with loose HMA.

Method 2 - Obtaining a Sample on Asphalt Surface:

1. After the paving machine has passed the sampling point, immediately place the “cookie cutter” sampling device on the location to be sampled. Push the cutter down through the HMA until it is flat against the underlying asphalt mat.
2. Using a small square tipped shovel and/or scoop, carefully remove all the HMA from inside of the cutter and place in a sample container. The hole made from the sampling must be filled by the contractor with loose HMA.

Identification and Shipping

1. Identify sample containers as required by the agency.
2. Ship samples in containers that will prevent loss, contamination, or damage.

Addendum WAQTC FOP for AASHTO T 168

Following are guidelines for the use of WAQTC FOP for AASHTO T 168 by the State of Alaska DOT&PF.

1. ATM 403 contains additional sampling methods.
2. When sampling asphalt mixture from a mat after compaction, sample in accordance with Section 413, WAQTC TM 11, “Sampling Bituminous Material after Compaction (Obtaining Cores).”

This page intentionally left blank.

Sampling Hot Mix Asphalt ATM 403

1. Scope

This method describes the procedures used for sampling Hot Mix Asphalt (HMA).

2. Significance and Use

This method provides procedures for sampling HMA in the field.

- 2.1. Sampling is equally as important as the testing, and the sampler shall use every precaution to obtain samples that will yield an acceptable estimate of the nature and conditions of the materials for which they represent.
- 2.2. Care shall be taken in sampling to avoid segregation of the material being sampled, and to prevent contamination by dust or other foreign matter.
- 2.3. If material is sampled by other than DOT&PF personnel or their agent(s), the sampling must be witnessed and possession of the sample transferred immediately to DOT&PF personnel or their agent(s).

3. Equipment

- 3.1 Flat scoop with vertical sides or a square point shovel
- 3.2 Plate with small lip (approximately ½") and of sufficient size and rigidity to accommodate required sample. Plate to have wire(s) attached to allow the plate to be located and removed from the mat after paver travels past it.
- 3.3 Approved sample containers including new cardboard boxes, clean metal buckets, cans or bowls.
- 3.4 Miscellaneous tools, scraper, scoop, gloves, etc.

4. Sampling from the Auger

- 4.1 Obtain samples from the accessible portion of the auger, using a square point shovel.
- 4.2 Place the shovel in front of the auger, with the blade flat upon the surface to be paved.
- 4.3 Allow the front face of the HMA coming off the auger to cover the shovel. Remove the shovel before the auger reaches the shovel by lifting it upward as vertically as possible being careful not to lose material.
- 4.4 Repeat the procedure at least three times, but as many times as necessary to obtain a sample of the required size.
- 4.5 Place the sample in an approved container for transport to Lab.

5. Lipped Plate Sampling

- 5.1 When using a pickup machine:
 - 5.1.1 Stop the paver and pickup machine.
 - 5.1.2 Place plate(s) underneath the pickup machine, midway between and just behind the rear tires and right in front of the paver.
- 5.2 When using dump trucks:
 - 5.2.1 Stop the paver after the truck is attached to the paver.
 - 5.2.2 Place plate(s) at the midpoint of the axis of the paver and behind the truck tires.

Note: when placing plate(s), avoid influence from truck tires, pickup machine tires, and paver tracks or tires.

- 5.3. Run an attached wire perpendicular to the direction of the paver, beyond the farthest auger extension and/or the ski.
 - 5.4. Hold the wire to the ground with your foot.
 - 5.5. Allow the paving operation to resume.
 - 5.6. When the paver has passed over the plate position, pull up on the wire to locate the plate. Remove the plate(s) laden with mix from the HMA mat by lifting vertically being careful not to disturb the mix at the edge of the plate.
 - 5.7. Place the entire sample in an approved container(s) for transport to the Lab.
- Note: make sure to hold the wire down on the ground so the ski will not snag it.

6. Windrow Sampling

- 6.1 Sample from the windrow created by a single truck. Divide the windrow length into three sections. Sample from three locations along the top of the middle section.
- 6.2 At each of the three locations in the middle section, remove and discard the top 12 inches. Remove a sample increment by digging vertically down with a square point shovel. Repeat for each increment.
- 6.3 Combine the three increments to form the composite sample.
- 6.4 Place the sample in an approved container for transport to the Lab.

REDUCING SAMPLES OF HOT MIX ASPHALT (HMA) TO TESTING SIZE FOP FOR AASHTO R 47 (See Addendum for DOT&PF Guidelines)

Significance

Samples of bituminous paving mixes taken in accordance with the FOP for AASHTO T 168 are composites and typically large in size. Materials sampled in the field need to be reduced to appropriate sizes for testing. As a general rule, field samples should be of a size that splitting once will result in the required test sample size. It is extremely important that the procedure used to reduce the field sample not modify the material properties.

Scope

This procedure covers sample reduction of Hot Mix Asphalt (HMA) to testing size. The reduced portion is to be representative of the original sample.

Apparatus

- Thermostatically controlled oven capable of maintaining a temperature of at least 110°C (230°F) or high enough to heat the material to a pliable condition for splitting.
- Non-contact temperature measuring device.
- Metal spatulas, trowels, metal straightedges, and/or drywall taping knives; for removing HMA samples from the quartering device, cleaning surfaces used for splitting, etc.
- Square-tipped, flat-bottom scoop, shovel or trowel for mixing HMA prior to quartering.
- Miscellaneous equipment including hot plate, non-asbestos heat-resistant gloves or mittens, pans, buckets, and cans.
- Sheeting: Non-stick heavy paper, heat-resistant plastic, or other material as approved by the agency.
- Agency-approved release agent, free of solvent or petroleum-based products that could affect asphalt binder properties.
- Mechanical Splitter Type A (Quartermaster): having four equal-width chutes discharging into four appropriately sized sample receptacles. Splitter is to be equipped with a receiving hopper that will hold the sample until the release lever is activated with four sample receptacles of sufficient capacity to accommodate the reduced portion of the HMA sample from the mechanical splitter. Refer to AASHTO R 47, Figures 1 through 3, for configuration and required dimensions of the mechanical splitter.
- Mechanical Splitter Type B (Riffle): having a minimum of eight equal-width chutes discharging alternately to each side with a minimum chute width of at least 50% larger than the largest particle size. A hopper or straight-edged pan with a width equal to or slightly smaller than the assembly of chutes in the riffle splitter to permit uniform discharge of the HMA through the chutes without segregation or loss of material. Sample receptacles of sufficient width and capacity to receive the reduced portions of HMA from the riffle splitter without loss of material.

- **Quartering Template:** formed in the shape of a cross with equal length sides at right angles to each other. Template shall be manufactured of metal that will withstand heat and use without deforming. The sides of the quartering template should be sized so that the length exceeds the diameter of the flattened cone of HMA by an amount allowing complete separation of the quartered sample. Height of the sides must exceed the thickness of the flattened cone of HMA.
- **Non-stick mixing surface** that is hard, heat-resistant, clean, level, and large enough to permit HMA samples to be mixed without contamination or loss of material.

Sampling

Obtain samples according to the FOP for AASHTO T 168.

Sample Preparation

The sample must be warm enough to separate. If not, warm in an oven until it is sufficiently soft to mix and separate easily. Do not exceed either the temperature or time limits specified in the test method(s) to be performed.

Selection of Procedure (Method)

Refer to agency requirements when determining the appropriate method(s) of sample reduction. In general, the selection of a particular method to reduce a sample depends on the initial size of the sample vs. the size of the sample needed for the specific test to be performed.

It is recommended that, for large amounts of material, the initial reduction be performed using a mechanical splitter. This decreases the time needed for reduction and minimizes temperature loss. Further reduction of the remaining HMA may be performed by a combination of the following methods, as approved by the agency. The methods for reduction are:

- **Mechanical Splitter Method**
 - Type A (Quartermaster)
 - Type B (Riffle Splitter)
- **Quartering Method**
 - Full Quartering
 - By Apex
- **Incremental (Loaf) Method**

Procedure

Mechanical Splitter Type A (Quartermaster)



Figure 1

1. Clean the splitter and apply a light coating of approved release agent to the surfaces that will contact HMA.
2. Close and secure hopper gates.
3. Place the four sample receptacles in the splitter so that there is no loss of material.
4. Remove the sample from the agency-approved container(s) and place the heated sample in the mechanical splitter hopper. Avoid segregation, loss of HMA or the accidental addition of foreign material.
5. Release the handle, allowing the HMA to drop through the divider chutes and discharge into the four receptacles.
6. Any HMA that is retained on the surface of the splitter shall be removed and placed into the appropriate receptacle.
7. Close and secure the hopper gates.
8. Reduce the remaining HMA as needed by this method or a combination of the following methods as approved by the agency.
9. Combine the material contained in the receptacles from opposite corners and repeat the splitting process until an appropriate sample size is obtained.
10. Retain and properly identify the remaining unused portion of the HMA sample for further testing if required by the agency.

Mechanical Splitter Type B (Riffle)



Figure 2

1. If heating of the testing equipment is desired, it shall be heated to a temperature not to exceed 110 °C (230°F).
2. Clean the splitter and apply a light coating of approved release agent to the surfaces that will come in contact with HMA (hopper or straight-edged pan, chutes, receptacles).
3. Place two empty receptacles under the splitter.
4. Carefully empty the heated HMA from the agency-approved container(s) into the hopper or straight-edged pan without loss of material. Uniformly distribute from side to side of the hopper or pan.
5. Discharge the HMA at a uniform rate, allowing it to flow freely through the chutes.
6. Any HMA that is retained on the surface of the splitter shall be removed and placed into the appropriate receptacle.
7. Reduce the remaining HMA as needed by this method or a combination of the following methods as approved by the agency.
8. Using one of the two receptacles containing HMA, repeat the reduction process until the HMA contained in one of the two receptacles is the appropriate size for the required test.
9. After each split, remember to clean the splitter hopper and chute surfaces if needed.
10. Retain and properly identify the remaining unused HMA sample for further testing if required by the agency.

Quartering Method

1. Heat all of the testing equipment (quartering template, scoop or trowel) to a temperature not to exceed 110 °C (230°F).
2. If needed, apply a light coating of release agent to quartering template.
3. Dump the heated sample from the agency approved container(s) into a conical pile on a hard, “non-stick”, clean, level surface where there will be neither a loss of material nor the accidental addition of foreign material. The surface can be made non-stick by the application of an approved asphalt release agent, or sheeting.

4. Mix the material thoroughly by turning the entire sample over a minimum of four times with a flat-bottom scoop; or by alternately lifting each corner of the sheeting and pulling it over the sample diagonally toward the opposite corner, causing the material to be rolled. Create a conical pile by either depositing each scoop or shovelful of the last turning on top of the preceding one, or lifting both opposite corners.
5. Flatten the conical pile to a uniform diameter and thickness where the diameter is four to eight times the thickness. Make a visual observation to ensure that the material is homogeneous.
6. Divide the flattened cone into four equal quarters using the quartering template. Press the template down until it is in complete contact with the surface on which the sample has been placed, assuring complete separation.

Note 1: Straightedges may be used in lieu of the quartering device to completely separate the material in approximately equal quarters.

7. Reduce the sample by quartering the sample completely or by removing the sample from the apex.
8. Full Quartering

- 8a. Remove two diagonally opposite quarters, including all of the fine material.
- 8b. Remove the quartering template and combine the remaining quarters, again forming a conical pile.
- 8c. Repeat steps 4, 5, 6, 8a, & 8b until a sample of the required size has been obtained. The final sample must consist of the two remaining diagonally opposite quarters.
- 8d. Retain and properly identify the remaining unused portion of the HMA sample for further testing if required by the agency.

9. By Apex

- 9a. Using a straightedge, slice through a quarter of the HMA from the center point to the outer edge of the quarter.
- 9b. Pull or drag the material from the quarter, holding one edge of the straightedge in contact with quartering device.
- 9c. Remove an equal portion from the opposite quarter and combine these increments to create the required sample size.

Note 2: Two straightedges may be used in lieu of the quartering device.

- 9d. Continue using the apex method with the unused portion of the HMA until samples have been obtained for all required tests.
- 9e. Retain and properly identify the remaining unused portion of the HMA sample for further testing if required by the agency.

Incremental Method (Loaf)

1. Cover a hard, clean, level surface with sheeting. This surface shall be large enough that there will be neither a loss of material nor the accidental addition of foreign material.
2. Place the sample from the agency approved container(s) into a conical pile on that surface.

3. Mix the material thoroughly by turning the entire sample over a minimum of four times with a flat-bottom scoop; or by alternately lifting each corner of the sheeting and pulling it over the sample diagonally toward the opposite corner, causing the material to be rolled. Create a conical pile by either depositing each scoop or shovelful of the last turning on top of the preceding one, or lifting both opposite corners.
4. Grasp the sheeting and roll the conical pile into a cylinder (loaf), then flatten the top. Make a visual observation to determine that the material is homogenous.
5. Pull the sheeting so at least $\frac{1}{4}$ of the length of the loaf is off the edge of the counter. Allow this material to drop into a container to be saved. As an alternate, using a straightedge, slice off approximately $\frac{1}{4}$ of the length of the loaf and place in a container to be saved.
6. Pull material (loaf) off the edge of the counter and drop into an appropriate size sample pan or container for the test to be performed. Continue removing material from the loaf until the proper size sample has been acquired. As an alternate, using a straightedge, slice off an appropriate size sample from the length of the loaf and place in a sample pan or container.
7. Repeat step 6 until all the samples for testing have been obtained.

***Note 3:** When reducing the sample to test size it is advisable to take several small increments, determining the mass each time until the proper minimum size is achieved. Unless the sample size is grossly in excess of the minimum or exceeds the maximum test size, use the sample as reduced for the test.*

Sample Identification

1. Identify the sample as required by the agency.
2. Samples shall be submitted in agency approved containers and secured to prevent contamination and spillage.

Addendum FOP for AASHTO R 47

Following are guidelines for the use of FOP for AASHTO R 47 by the State of Alaska DOT&PF.

1. The incremental method may be done without sheeting.
2. Unless specifically allowed by project specifications, the mechanical splitter method(s) are not allowed.

This page intentionally left blank.

Asphalt Cement Content of Hot Mix Asphalt by the Nuclear Method

ATM 405

1. Scope

This method covers the quantitative determination of the asphalt cement content of Hot Mix Asphalt by testing a sample with a device that utilizes neutron thermalization techniques. This is an adaptation of AASHTO T 287. Job mix design (JMD) calibration, cross calibration of master and field gauges and calibration transfer are included.

2. Referenced Documents

- WAQTC Standards:
 - FOP for AASHTO T 2, Sampling of Aggregates
 - FOP for AASHTO T 168, Sampling Bituminous Paving Mixtures
 - FOP for AASHTO R47, Reducing Samples of Hot Mix Asphalt to Testing Size
 - FOP for AASHTO T 329, Moisture Content of Bituminous Mixes by Oven
- Other Documents:
 - Manufacturer's instruction manual.

3. Significance and Use

This method can be used for rapidly determining the asphalt content of HMA. Testing can be completed in a matter of minutes so that adjustments, if necessary, can be made in the asphalt metering system with a limited amount of mix production. The procedure is useful in the determination of asphalt content only, as it does not provide extracted aggregate for the gradation analysis.

4. Apparatus

- Nuclear asphalt content gauge system consisting of:
 - Neutron source: an encapsulated and sealed radioactive source
 - Thermal neutron detectors
 - Read-out instrument displaying, at a minimum, percent asphalt cement
 - Two or more stainless steel sample pans conforming to gauge requirements
- Sample containers with lids or other methods of closing to prevent contamination and of sufficient size to hold the entire sample. The containers should be able to withstand the reheating of the mix to mixing temperature.
- Sample quartering apparatus conforming to requirements of the WAQTC FOP for AASHTO R 47.
- Balance or scale: capable of determining mass to 15 kg, readable to 1 g and conforming to AASHTO M 231.
- Drying oven, of either of the following types, capable of handling the volume and sample size expected for the project:
 - Forced air, ventilated or convection oven capable of maintaining a temperature of $177 \pm 3^{\circ}\text{C}$ ($350 \pm 5^{\circ}\text{F}$)
 - Leveling plate: Flat, rigid plate of metal with a minimum thickness of 10 mm ($\frac{3}{8}$ in) and slightly larger than the sample pans
 - Thermometer with a temperature range of 10-300°C (50-500°F)
 - Assorted pans, spoons, spatulas, and mixing bowls

- Radioactive materials information and calibration packet containing:
- Daily Background Count Log
- Leak Test Certificate
- Shippers Declaration for Dangerous Goods
- Procedure Memo for Storing, Transporting and Handling Nuclear Testing Equipment
- Other radioactive materials documentation as required by local regulatory requirements

5. Precautions

1. The equipment shall be so constructed as to be licensable in accordance with applicable health and safety regulations.
2. Equipment operators shall wear an approved form of radiation dosimetry (i.e., film badges, thermo luminescent dosimeter, etc) capable of monitoring the occupational radiation exposure.
3. Since nuclear equipment measures the total amount of hydrogen in the sample, this procedure is sensitive to changes in moisture content. It must be remembered that both asphalt cement and water contain hydrogen.
4. Keep any other source of neutron radiation at least 10 m (30 ft) from the equipment. Do not place the equipment where large amounts of hydrogenous material may be moved during the calibration or testing procedures (for example, water or plastic materials).
5. All personnel shall be kept at least 1 m (3 ft) away from the gauge during testing.

6. Standardization

1. Obtain and record a 16 minute background count, in accordance with manufacturer's procedure, each day prior to taking test measurements or whenever the gauge has been moved or the conditions within 1 m (3 ft) of the gauge have changed. The measurement time for the background count is the same as that used for test measurements.
2. If the background count has not changed by more than 2 percent from the previous background count, then the apparatus shall be considered stable and acceptable for use. If the gauge has been moved or if the surrounding conditions have changed, additional background counts must be obtained until the 2 percent standard is met.

7. Calibration

1. This method is sensitive to the type of aggregate, percentage and source of asphalt cement, and to the aggregate gradation. Accordingly, a calibration curve must be developed for each mix type. When changes occur, a new calibration should be run. The curve shall be established with 3 points. (See Appendix A)
2. Prior to the start of each test, verify that the activated calibration is correct.

8. Procedure

1. Determine the mass of a clean gauge sample pan, and use this to determine the sample mass in the pan, or tare the pan on the scale.
2. Using a hot asphalt concrete mixture sample having a temperature of 121° to 149°C (250° to 300°F) obtained in accordance with WAQTC FOP for AASHTO T 168, and reduced in accordance with WAQTC FOP for AASHTO R 47, fill the sample pan one-half full, evenly distributing the sample in the pan. Level the asphalt concrete mixture with a preheated trowel or spatula, spading as necessary to compact (usually 10 to 15 spades are sufficient), being careful to avoid segregating the mix or driving the fines into the bottom.

3. Fill the remainder of the pan until the mass of the asphalt concrete mixture in the pan is approximately equal to or up to 5 grams above the mass of mix used for the calibration samples. Level the top of the asphalt concrete mixture using a spatula or trowel and spade as necessary to compact (usually 10 to 15 spades are sufficient), avoiding segregation of the mix. Compact the sample into the pan, until it is level with the top of the pan, by standing on the metal plate and rocking/twisting back-and-forth.
4. Verify that the mass of mix is ± 5 g of the calibration mass. Record the mass of the asphalt concrete mixture in the pan.
5. If the gauge does not have temperature compensation capability, measure and record the temperature of the compacted specimen. This temperature must be within $\pm 5^{\circ}\text{C}$ ($\pm 9^{\circ}\text{F}$) of the calibration test specimen temperature.
6. Place the pan into the gauge. Perform a 16 minute count.
7. Determine and record the uncorrected asphalt cement content to the nearest 0.01 percent by direct readout from the gauge, from the calibration graph, or by the formula supplied by the manufacturer.
8. Using a representative portion of the original sample or a portion of the material removed from the gauge pan, determine the moisture in the mixture in accordance with the WAQTC FOP for AASHTO T 329 and record to the nearest 0.01 percent.

Note 1: When taking the moisture from the gauge pan sample, remove it immediately after completing the oil content test.

9. Calculation

1. Subtract the moisture content from the uncorrected asphalt cement content. Record this as the corrected asphalt cement content.

10. Report

Results shall be reported on standard forms approved by the agency. Report the following information.

- Make, model, and serial number of the nuclear asphalt content gauge.
- Date and source of calibration.
- Date of test.
- Name and signature of operator.
- Background count for the day of the test.
- Mix identification.
- Aggregate type and source(s); Asphalt cement source, type and grade.
- Calibration sample mass and temperature.
- Test sample mass and temperature, if gauge does not have temperature compensation capability
- Gauge reading, including print-out from gauge.
- Asphalt cement content value to the nearest 0.1 %.
- Attach the Nuclear Gauge print out to the report.

Appendix A ATM 405

1. Gauge Calibration

1. Obtain samples of aggregate in accordance with WAQTC FOP for AASHTO T 2. Approximately 50 kg (110 lb) total will be required for calibration specimens. Dry the aggregates in accordance with WAQTC FOP for AASHTO T 255/T 265, separate into sieve sizes determined by the JMD.
2. Blend the aggregate together at the proper proportion to match the job mix formula following steps 3 and 4.
3. Calculate the required cumulative mass for each specified sieve using the following formula:

$$X = \frac{(100 - P)}{100} \times T$$

where:

X = Required cumulative batch mass for each specified sieve

P = Percent passing for each specified sieve according to the job mix formula

T = Initial total aggregate mass

4. Correct for aggregate dust as follows.
 - a. Prepare a wash gradation sample from the mass calculated in Step 4.
 - b. Perform a washed gradation following WAQTC FOP for AASHTO T 27/T 11.
 - c. Compute the corrected batch mass for each specified sieve for the calibration points using the following formula:

$$Z_n = \frac{X^2}{Y}$$

where:

Z_n = Adjusted cumulative batch mass for sieve size n.

X = Pre-wash cumulative batch mass for each specified sieve.

Y = Post-wash cumulative batch mass for each specified sieve.

5. Obtain samples of bituminous materials in accordance with WAQTC FOP for AASHTO T 40. Approximately 4 L (1 gal) will be required.
6. Calculate the mass of asphalt cement for each calibration point as follows:

$$B = E \times P_{bm}$$

where:

B = mass of asphalt cement to the nearest 0.1 g

E = mass of mix

P_{bm} = percent asphalt cement content by total mass of mixture, expressed as a decimal.

7. Use the three following asphalt cement contents:
 - Specified minus 1.0 percent
 - Specified (mix design value)
 - Specified plus 1.0 percent

8. Calculate the mass of aggregate required for each calibration point as follows:

$$A = E - B$$

where:

- A = mass of aggregate to the nearest 0.1 g
- B = mass of asphalt cement to the nearest 0.1 g
- E = mass of mix

2. Preparation of Calibration Specimens

1. Heat the prepared aggregate specimens to the mixing temperature range midpoint for the asphalt cement $\pm 5^{\circ}\text{C}$ ($\pm 9^{\circ}\text{F}$) and hold at that temperature for three hours or to constant mass.
2. Heat the asphalt cement to the mid-point of the mixing temperature range $\pm 5^{\circ}\text{C}$ ($\pm 9^{\circ}\text{F}$) in a covered container(s). It is best to use the asphalt cement as soon as it reaches mixing temperature. If this is not possible, maintain the asphalt cement at this temperature, rather than cool and reheat it, but do not hold the sample at this temperature for more than 4 hours.
3. All bowls, sample pans, and tools should be heated to the mid-point of the mixing temperature range $\pm 5^{\circ}\text{C}$ ($\pm 9^{\circ}\text{F}$). An initial or “butter” mix is required to condition the mixing equipment. Mix a minimum of three asphalt concrete specimens to cover the approximate range of the design asphalt content. Mix one at the design asphalt content, one 1.0 percent above, and one 1.0 percent below, use the same grade and type of asphalt as will be used in the asphalt concrete mixture to be tested. Mix 7000-9000g for each specimen.
4. Fill the sample pan one-half full, evenly distributing the sample in the pan. Level the asphalt concrete mixture with a spatula or trowel and spade as necessary to compact, avoiding segregation of the mix. Fill the remainder of the pan until the asphalt concrete mixture is mounded slightly above the top of the pan. Record the weight of the asphalt concrete mixture in the pan. This is the weight that is to be used for all calibration and test samples using this calibration. Level the top of the asphalt concrete mixture using a spatula or trowel and spade as necessary to compact, avoiding segregation of the mix. Use the metal plate to consolidate the asphalt concrete mixture until it is level with the top edge of the pan. All specimens should be compacted at the mid-point of the mixing temperature range $\pm 5^{\circ}\text{C}$ ($\pm 9^{\circ}\text{F}$) to ensure that the mix will compact properly.
5. Place each calibration pan into the gauge and proceed in accordance with the manufacturer’s instructions for operation of the equipment and the sequence of operations. Count each calibration sample for 16 minutes.

Note: Do not forget to perform and record a background count as per the manufacturer’s instructions.

6. For gauges that generate the calibration internally, print out the formula coefficients (“A” Values), the coefficient of fit and the calculated percent difference for each calibration point. The coefficient of fit must be between 0.998 and 1.000 for dense graded mix or 0.995 and 1.000 for open graded mix. Calibration points must have a calculated percent difference of less than 0.09 percent. If either requirement is not met, the calibration must be redone.
7. Store the acceptable calibration in the gauge’s memory, using the job mix formula and the Contract number or an easily recognizable calibration number, according to the manufacturer’s instructions.
8. For gauges other than the Troxler, prepare a calibration curve by plotting the calibration sample gauge readings versus asphalt cement content on linear graph paper, choosing convenient scale factors for gauge readings and asphalt cement content.
9. Calculate the correlation factor for gauges without internal calculations according to the following formula:

$$CorrelationFactor = \sqrt{1 - \frac{\sum_i \left(Y_i - \hat{Y}_i \right)^2}{\sum_i \left(Y_i - \bar{Y}_i \right)^2}}$$

where:

Y_i = actual percent asphalt values for each sample

\hat{Y}_i = calculated percent asphalt values from curve

\bar{Y}_i = mean value of the actual percentages asphalt, and

i = number of calibration samples.

Appendix B ATM 405

1. Cross Calibration (Troxler 3241)

1. Cross calibrating creates a relationship between the field gauge and a master gauge. This allows testing of production mix with a field gauge without the need to perform physical calibrations. When several gauges are cross calibrated, the mix calibrations may be transferred to each. The master gauge is normally located where the calibration sample pans are fabricated.
2. The central lab shall prepare the cross calibration samples. Prepare six calibration samples, using a locally available specification aggregate, with binder contents between 3 and 8 percent at 1 percent increments or per the gauge manufacturer's instructions. Mix the samples so that each pan of mix equals the base mass ± 5 g. Run each sample in the master gauge using a 16 minute count in the normal calibration mode. After all samples are run, the gauge will automatically calculate a coefficient of fit. The coefficient of fit must be at least 0.999.
3. Seal each pan to prevent change in hydrogen content and repeat steps 1 and 2. Sealed pans must meet same criteria.
4. Run each of the six sealed calibration samples in the field gauge while in cross calibration mode utilizing a 16 minute count. For each calibration sample, input the information from the master gauge into the field gauge. When the six cross calibration samples have been counted, print out the cross calibration data. The coefficient of fit must be .999 or 1.000. If this requirement is met, the master gauge and the field gauge are cross calibrated.

2. Calibration Transfer

When the field gauge has been cross calibrated with the master gauge a calibration transfer can be performed. JMD calibrations can now be transferred to the field gauge, using input data only. This transfer would be in lieu of calibrating the field gauge with a JMD calibration. Follow the manufacturer's instructions to perform this transfer.

This page intentionally left blank.

PERFORMANCE EXAM CHECKLIST

ASPHALT BINDER CONTENT OF BITUMINOUS MIXTURES BY THE NUCLEAR METHOD ATM 405

Participant Name _____ Exam Date _____

Procedure Element	Trial 1	Trial 2
1. Precautions for gauge adequately described? Run background count?	_____	_____
2. Sample obtained as per AASHTO T 168? 250-300 degrees?	_____	_____
3. Sample reduced as per WAQTC FOP for AASHTO R 47?	_____	_____
4. First layer properly consolidated?	_____	_____
5. Second layer properly consolidated?	_____	_____
6. Sample compacted using the correct size leveling plate?	_____	_____
7. Mass checks within ± 5 g of base mass?	_____	_____
8. Temperature of mix recorded (if necessary)?	_____	_____
9. Correct calibration used?	_____	_____
10. 16 minute count taken and uncorrected binder content recorded to 0.01 percent?	_____	_____
11. Corrected binder content correctly determined and recorded to nearest 0.1 percent?	_____	_____

Comments: First trial: Pass ☐ Fail ☐ Second trial: Pass ☐ Fail ☐

Signature of Examiner _____

DETERMINING THE ASPHALT BINDER CONTENT OF HOT MIX ASPHALT (HMA) BY THE IGNITION METHOD (See Addendum for DOT&PF Guidelines) **WAQTC FOP FOR AASHTO T 308**

Scope

This procedure covers the determination of asphalt binder content of hot mix asphalt (HMA) by ignition of the binder at 538°C (1000°F) or less in a furnace; samples may be heated by convection or direct infrared irradiation (IR). The aggregate remaining after burning can be used for sieve analysis using the FOP for AASHTO T 30.

Two methods, A and B, are presented.

Some agencies allow the use of recycled HMA. When using recycled HMA, check with the agency for specific correction procedures.

Background on Test Method

Binder in the HMA is ignited in a furnace. Asphalt binder content is calculated as the difference between the initial mass of the HMA and the mass of the residual aggregate, correction factor, and moisture content. The asphalt binder content is expressed as percent of moisture-free mix mass.

Sampling

1. Obtain samples of HMA in accordance with the FOP for AASHTO T 168.
2. Reduce HMA samples in accordance with the FOP for AASHTO R 47.
3. If the mixture is not sufficiently soft to separate with a spatula or trowel, place it in a large flat pan in an oven at $125 \pm 5^{\circ}\text{C}$ ($257 \pm 9^{\circ}\text{F}$) until soft enough.
4. Test sample size shall conform to the mass requirement shown in Table 1.

Note 1: When the mass of the test specimen exceeds the capacity of the equipment used or for large samples of fine mixes, the test specimen may be divided into suitable increments, tested, and the results appropriately combined through a weighted average for calculation of the binder content.

Table 1

Nominal Maximum Aggregate Size* mm (in.)	Minimum Mass Specimen g	Maximum Mass Specimen g
37.5 (1 ½)	4000	4500
25.0 (1)	3000	3500
19.0 (¾)	2000	2500
12.5 (½)	1500	2000
9.5 (¾)	1200	1700
4.75 (No. 4)	1200	1700

* One sieve larger than the first sieve to retain more than 10 percent of the material using an agency specified set of sieves based on cumulative percent retained. Where large gaps in specification sieves exist, intermediate sieve(s) may be inserted to determine nominal maximum size.

Apparatus

Note 2: The apparatus must be calibrated for the specific mix design. See “Correction Factors” at the end of this FOP.

There are two methods – A and B. The apparatus for the two methods are the same except that the furnace for Method A has an internal balance.

- **Ignition Furnace:** A forced-air ignition furnace that heats the specimens by either the convection or direct IR irradiation method. The convection-type furnace must be capable of maintaining the temperature at 578°C (1072°F).

For Method A, the furnace will be equipped with an internal scale thermally isolated from the furnace chamber and accurate to 0.1 g. The scale shall be capable of determining the mass of a 3500 g sample in addition to the sample baskets. A data collection system will be included so that mass can be automatically determined and displayed during the test. The furnace shall have a built-in computer program to calculate the change in mass of the sample baskets and provide for the input of a correction factor for aggregate loss. The furnace shall provide a printed ticket with the initial specimen mass, specimen mass loss, temperature compensation, correction factor, corrected binder content, test time, and test temperature. The furnace shall provide an audible alarm and indicator light when the sample mass loss does not exceed 0.01% of the total sample mass for three consecutive minutes.

Note 3: The furnace shall be designed to permit the operator to change the ending mass loss percentage from 0.01 percent to 0.02 percent.

For both Method A and Method B, the furnace chamber dimensions shall be adequate to accommodate a 3500 g sample. The furnace door shall be equipped so that it cannot be opened during the ignition test. A method for reducing furnace emissions shall be provided and the furnace shall be vented so that no emissions escape into the laboratory. The furnace shall have a fan to pull air through the furnace to expedite the test and to eliminate the escape of smoke into the laboratory.

- **Sample Basket Assembly:** consisting of sample basket(s), catch pan, and basket guards. Sample basket(s) will be of appropriate size allowing samples to be thinly spread and allowing air to flow through and around the sample particles. Sets of two or more baskets shall be nested. A catch pan: of sufficient size to hold the sample basket(s) so that aggregate particles and melting binder falling through the screen mesh are caught. Basket guards will completely enclose the basket and be made of screen mesh, perforated stainless steel plate, or other suitable material.

Note 4: Screen mesh or other suitable material with maximum and minimum openings of 2.36 mm (No. 8) and 600 µm (No. 30) respectively has been found to perform well.

- Thermometer, or other temperature measuring device, with a temperature range of 10 -260°C (50-500°F).
- Oven capable of maintaining 125 ±5°C (257 ±9°F).
- Balance or scale: Capacity sufficient for the sample mass and conforming to the requirements of M 231, Class G2.
- **Safety equipment:** Safety glasses or face shield, high temperature gloves, long sleeved jacket, a heat resistant surface capable of withstanding 650°C (1202°F), a protective cage capable of surrounding the sample baskets during the cooling period, and a particle mask for use during removal of the sample from the basket assembly.

- Miscellaneous equipment: A pan larger than the sample basket(s) for transferring sample after ignition, spatulas, bowls, and wire brushes.

Procedure – Method A (Internal Balance)

1. For the convection-type furnace, preheat the ignition furnace to 538°C (1000°F) or to the temperature determined in the “Correction Factor” section, Step 9 of this method. Manually record the furnace temperature (set point) prior to the initiation of the test if the furnace does not record automatically. For the direct IR irradiation-type furnace, use the same burn profile as used during the correction factor determination.
2. Dry the sample to constant mass, according to the FOP for AASHTO T 329; or determine the moisture content of a companion sample in accordance with the FOP for AASHTO T 329.
3. Determine and record the mass to the nearest 0.1 g of the sample basket assembly.
4. Evenly distribute the sample in the sample basket assembly, taking care to keep the material away from the edges of the basket. Use a spatula or trowel to level the sample.
5. Determine and record the total mass of the sample and sample basket assembly to the nearest 0.1 g. Calculate and record the initial mass of the sample (total mass minus the mass of the sample basket assembly) to the nearest 0.1 g. Designate this mass as (M_i).
6. Record the correction factor or input into the furnace controller for the specific HMA.
7. Input the initial mass of the sample (M_i) into the ignition furnace controller. Verify that the correct mass has been entered.

CAUTION: operator should wear safety equipment – high temperature gloves, face shield, fire-retardant shop coat – when opening the door to load or unload the sample.

8. Open the chamber door and gently set the sample basket assembly in the furnace. Carefully position the sample basket assembly so it is not in contact with the furnace wall. Close the chamber door and verify that the sample mass displayed on the furnace scale equals the total mass of the sample and sample basket assembly recorded in Step 5 within ± 5 g.

Note 5: Furnace temperature will drop below the set point when the door is opened, but will recover when the door is closed and ignition begins. Sample ignition typically increases the temperature well above the set point – relative to sample size and binder content.

9. Initiate the test by pressing the start button. This will lock the sample chamber and start the combustion blower.

Safety note: Do not attempt to open the furnace door until the asphalt binder has been completely burned off.

10. Allow the test to continue until the stable light and audible stable indicator indicate that the change in mass does not exceed 0.01% for three consecutive minutes. Press the stop button. This will unlock the sample chamber and cause the printer to print out the test results.

Note 6: An ending mass loss percentage of 0.02 may be used, if allowed by the agency, when aggregate that exhibits an excessive amount of loss during ignition testing is used

11. Open the chamber door, remove the sample basket assembly, and place on the cooling plate or block. Place the protective cage over the sample basket assembly and allow it to cool to room temperature (approximately 30 minutes).

12. Determine and record the total after ignition mass to the nearest 0.1 g. Calculate and record the mass of the sample, after ignition (total after ignition mass minus the mass of the sample basket assembly) to the nearest 0.1 g. Designate this mass as M_f .
13. Use the asphalt binder content percentage from the printed ticket. Subtract the moisture content from the printed ticket asphalt binder content and report the difference as the corrected asphalt binder content.

$$P_b = BC - MC - C_f \text{ (if not input in the furnace controller)}$$

where:

P_b = the corrected asphalt binder content as a percent by mass of the HMA

BC = asphalt binder content shown on printed ticket

MC = moisture content of the companion HMA sample, percent, as determined by the FOP for AASHTO T 329 (if the specimen was oven-dried prior to initiating the procedure, $MC=0$)

C_f = correction factor as a percent by mass of the HMA sample

14. Asphalt binder content percentage can also be calculated using the formula from “Method B” Step 16.

Procedure – Method B (External Balance)

1. Preheat the ignition furnace to 538°C (1000°F) or to the temperature determined in the “Correction Factor” section (Step 9). Manually record the furnace temperature (set point) prior to the initiation of the test if the furnace does not record automatically.
2. Dry the sample to constant mass, according to the FOP for AASHTO T 329; or determine the moisture content of a companion sample in accordance with the FOP for AASHTO T 329.
3. Determine and record the mass of the sample basket assembly to the nearest 0.1 g.
4. Place the sample basket(s) in the catch pan. Evenly distribute the heated sample in the sample basket(s), taking care to keep the material away from the edges of the basket. Use a spatula or trowel to level the sample.
5. Determine and record the total mass of the sample and sample basket assembly to the nearest 0.1 g. Calculate and record the initial mass of the sample (total mass minus the mass of the sample basket assembly) to the nearest 0.1 g. Designate this mass as (M_i).
6. Record the correction factor for the specific HMA.
7. Open the chamber door and gently set the sample basket assembly in the furnace. Carefully position the sample basket assembly so it is not in contact with the furnace wall. Burn the HMA sample in the furnace for 45 minutes or the length of time determined in the “Correction Factors” section.
8. Open the chamber door, remove the sample basket assembly, and place on the cooling plate or block. Place the protective cage over the sample and allow it to cool to room temperature (approximately 30 min).
9. Determine and record the total after ignition mass to the nearest 0.1 g. Calculate and record the mass of the sample, after ignition (total after ignition mass minus the mass of the sample basket assembly) to the nearest 0.1 g.
10. Place the sample basket assembly back into the furnace.

11. Burn the sample for at least 15 minutes after the furnace reaches the set temperature.
12. Open the chamber door, remove the sample basket assembly, and place on the cooling plate or block. Place the protective cage over the sample basket assembly and allow it to cool to room temperature (approximately 30 min.).
13. Determine and record the total after ignition mass to the nearest 0.1 g. Calculate and record the mass of the sample, after ignition (total after ignition mass minus the mass of the sample basket assembly) to the nearest 0.1 g.
14. Repeat Steps 10 through 13 until the change in measured mass of the sample after ignition does not exceed 0.01 percent of the previous sample mass after ignition.

Note 6: An ending mass loss percentage of 0.02 may be used, if allowed by the agency, when aggregate that exhibits an excessive amount of loss during ignition testing is used.

15. Record the final value obtained as M_f , the final mass of the sample after ignition.
16. Calculate the asphalt binder content of the sample as follows:

$$P_b = \left[\frac{M_i - M_f}{M_i} \right] \times 100 - C_f - MC$$

where:

P_b = the corrected asphalt binder content as a percent by mass of the HMA sample

M_f = the final mass of aggregate remaining after ignition

M_i = the initial mass of the HMA sample prior to ignition

C_f = correction factor as a percent by mass of the HMA sample

MC = moisture content of the companion HMA sample, percent, as determined by the FOP for AASHTO T 329 (if the specimen was oven-dried prior to initiating the procedure, $MC=0$).

Gradation

1. Empty contents of the basket(s) into a flat pan, being careful to capture all material. Use a small wire brush to ensure all residual fines are removed from the baskets.

Note 7: Particle masks are a recommended safety precaution.

2. Perform the gradation analysis in accordance with the FOP for AASHTO T 30.

Report

Results shall be reported on standard forms approved by the agency. Include:

- Method of test (A or B)
- Corrected asphalt binder content, P_b , per agency standard
- Correction factor, C_f , to 0.01%
- Temperature compensation factor (if applicable)
- Total percent loss
- Sample mass
- Moisture content to 0.01%

- Test temperature

Attach the original printed ticket with all intermediate values (continuous tape) to the report for furnaces with internal balances.

Correction Factors

Asphalt Binder and Aggregate

Asphalt binder content results may be affected by the type of aggregate in the mixture and by the ignition furnace. Asphalt binder and aggregate correction factors must, therefore, be established by testing a set of correction specimens for each Job Mix Formula (JMF) mix design. Each ignition furnace will have its own unique correction factor determined in the location where testing will be performed.

This procedure must be performed before any acceptance testing is completed, and repeated each time there is a change in the mix ingredients or design. Any changes greater than 5% in stockpiled aggregate proportions should require a new correction factor.

All correction samples will be prepared by a central / regional laboratory unless otherwise directed.

Asphalt binder correction factor: A correction factor must be established by testing a set of correction specimens for each Job Mix Formula (JMF). Certain aggregate types may result in unusually high correction factors ($> 1.00\%$). Such mixes should be corrected and tested at a lower temperature as described below.

Aggregate correction factor: Due to potential aggregate breakdown during the ignition process, a correction factor will need to be determined for the following conditions:

- a. Aggregates that have a proven history of excessive breakdown
- b. Aggregate from an unknown source.

This correction factor will be used to adjust the acceptance gradation test results obtained according to the FOP for AASHTO T 30.

Procedure

1. Obtain samples of aggregate in accordance with the FOP for AASHTO T 2.
 2. Obtain samples of asphalt binder in accordance with the FOP for AASHTO T 40.
- Note 8:* Include other additives that may be required by the JMF.
3. Prepare an initial, or “butter,” mix at the design asphalt binder content. Mix and discard the butter mix prior to mixing any of the correction specimens to ensure accurate asphalt content.
 4. Prepare two correction specimens at the JMF design asphalt binder content. Aggregate used for correction specimens shall be sampled from material designated for use on the project. An agency approved method will be used to combine aggregate. An additional “blank” specimen shall be batched and tested for aggregate gradation in accordance with the FOP for AASHTO T 30. The gradation from the “blank” shall fall within the agency specified mix design tolerances.
 5. Place the freshly mixed specimens directly into the sample basket assembly. If mixed specimens are allowed to cool prior to placement in the sample basket assembly, the specimens must be dried to constant mass according to the FOP for AASHTO T 329. Do not preheat the sample basket assembly.
 6. Test the specimens in accordance with Method A or Method B of the procedure.
 7. Once both of the correction specimens have been burned, determine the asphalt binder content for each specimen by calculation or from the printed oven tickets, if available.

8. If the difference between the asphalt binder contents of the two specimens exceeds 0.15%, repeat with two more specimens and, from the four results, discard the high and low result. Determine the correction factor from the two original or remaining results, as appropriate. Calculate the difference between the actual and measured asphalt binder contents for each specimen to 0.01%. The asphalt binder correction factor, C_f , is the average of the differences expressed as a percent by mass of HMA.
 9. If the asphalt binder correction factor exceeds 1.00%, the test temperature must be lowered to $482 \pm 5^\circ\text{C}$ ($900 \pm 8^\circ\text{F}$) and new samples must be burned.
 10. For the direct IR irradiation-type burn furnaces, the **default** burn profile should be used for most materials. The operator may select burn-profile **Option 1** or **Option 2** to optimize the burn cycle. Option 1 is designed for aggregate that requires a large aggregate correction factor (greater than 1 percent) – typically very soft aggregate (such as dolomite). Option 2 is designed for samples that may not burn completely using the **default** burn profile. The burn profile for testing HMA samples shall be the same burn profile selected for correction samples.
- Note 9:** The temperature for determining the asphalt binder content of HMA samples by this procedure shall be the same temperature determined for the correction samples.
11. Perform a gradation analysis on the residual aggregate in accordance with the FOP for AASHTO T 30, if required. The results will be utilized in developing an “Aggregate Correction Factor” and should be calculated and reported to 0.1%.
 12. From the gradation results subtract the percent passing for each sieve, for each sample, from the percent passing each sieve of the “Blank” specimen gradation results from Step 4.
 13. Determine the average difference of the two values. If the difference for any single sieve exceeds the allowable difference of that sieve as listed in Table 2, then aggregate gradation correction factors (equal to the resultant average differences) for all sieves shall be applied to all acceptance gradation test results determined by the FOP for AASHTO T 30. If the 75 μm (No. 200) is the only sieve outside the limits in Table 2, apply the aggregate correction factor to only the 75 μm (No. 200) sieve.

Table 2
Permitted Sieving Difference

Sieve	Allowable Difference
Sizes larger than or equal to 2.36 mm (No.8)	$\pm 5.0\%$
Sizes larger than to 75 μm (No.200) and smaller than 2.36 mm (No.8)	$\pm 3.0\%$
Sizes 75 μm (No.200) and smaller	$\pm 0.5\%$

Addendum WAQTC FOP for AASHTO T 308

Following are guidelines for the use of WAQTC FOP for AASHTO T 308 by the State of Alaska DOT&PF.

1. Delete Step 9 in Correction Factors – Procedure.
2. Unless otherwise specified, Method A (using step 14 calculation) shall be used.
3. Asphalt binder content shall be calculated with masses determined on an external balance. This applies to all test samples as well as calibration samples.
4. Nominal Maximum size shall be determined by the Job Mix Formula target value gradation.
5. Determine M_f approximately 30 minutes after removing from oven. M_f shall be determined no later than 3 hours after removal from oven.
6. Corrected asphalt binder content reported to 0.1%.
7. Use of the printed ticket is optional.

This page intentionally left blank.

MOISTURE CONTENT OF HOT MIX ASPHALT (HMA) BY OVEN METHOD FOP FOR AASHTO T 329

Scope

This procedure covers the determination of moisture content of HMA in accordance with AASHTO T 329.

Summary

A test specimen of HMA is dried in a forced-air ventilated or convection oven to constant mass.

Apparatus

- Balance or scale: 2 kg (4.4 lb) capacity, readable to 0.1 g and conforming to AASHTO M 231.
- Forced-air, ventilated, or convection oven: Capable of maintaining the temperature surrounding the sample at $163 \pm 14^{\circ}\text{C}$ ($325 \pm 25^{\circ}\text{F}$).
- Sample Container: Clean, dry, not affected by heat and of sufficient size to contain a test sample without danger of spilling .
- Thermometer or other suitable device with a temperature range of $10\text{-}260^{\circ}\text{C}$ ($50\text{-}500^{\circ}\text{F}$).

Sample

The test sample shall be obtained in accordance with the FOP for AASHTO T 168, and reduced in accordance with the FOP for AASHTO R 47. The size of the test sample shall be a minimum of 1000 g.

Procedure

1. Preheat the oven to a minimum of 105°C (221°F), but do not exceed the Job Mix Formula (JMF) mixing temperature. If the mixing temperature is not supplied, a temperature of $163 \pm 14^{\circ}\text{C}$ ($325 \pm 25^{\circ}\text{F}$) is to be used.
Note 1: For repeatability between laboratories, the preferred practice is to dry the sample at no less than 9°C (15°F) below the JMF mixing temperature.
2. Determine and record the mass of the sample container, including release media, to the nearest 0.1 g.
3. Place the test sample in the sample container.
4. Determine and record the temperature of the test sample.
- 5.
6. Determine and record the total mass of the sample container and test sample to the nearest 0.1 g.
6. Calculate the initial, moist mass (M_i) of the test sample by subtracting the mass of the sample container as determined in Step 2 from the total mass of the sample container and the test sample as determined in Step 5.
7. The test sample shall be initially dried for 90 ± 5 minutes, and its mass determined. Then it shall be dried at 30 ± 5 min intervals until constant mass is achieved.

Note 2: Constant mass shall be defined as the mass at which further drying does not alter the mass by more than 0.05 percent.

8. Cool the sample container and test sample to $\pm 9^{\circ}\text{C}$ (15°F) of the temperature determined in Step 4.
9. Determine and record the total mass of the sample container and test sample to the nearest 0.1 g.

Note 3: Do not attempt to remove the test sample from the sample container for the purposes of determining mass.

10. Calculate the final, dry mass (M_f) of the test sample by subtracting the mass of the sample container as determined in Step 2 from the total mass of the sample container and the test sample as determined in Step 9.

Note 4: Moisture content and the number of samples in the oven will affect the rate of drying at any given time. Placing wet samples in the oven with nearly dry samples could affect the drying process.

Calculations

Constant Mass:

Calculate constant mass using the following formula:

$$\% \text{ Change} = \frac{M_p - M_n}{M_p} \times 100$$

Where: M_p = previous mass measurement
 M_n = new mass measurement

Moisture Content:

Calculate the moisture content, as a percent, using the following formula.

$$\text{Moisture Content} = \frac{M_i - M_f}{M_f} \times 100$$

Where: M_i = initial, moist mass
 M_f = final, dry mass

Report

Results shall be reported on standard forms approved for use by the agency. Report the moisture content to 0.01 percent.

MECHANICAL ANALYSIS OF EXTRACTED AGGREGATE FOP FOR AASHTO T 30 (See Addendum for DOT&PF Guidelines)

Scope

This procedure covers mechanical analysis of aggregate recovered from bituminous mix samples in accordance with AASHTO T 30. This FOP utilizes the aggregate recovered from the ignition oven used in AASHTO T 308. AASHTO T 30 was developed for analysis of extracted aggregate and thus includes references to extracted bitumen and filter element, which do not apply in this FOP.

Sieve analyses determine the gradation or distribution of aggregate particles within a given sample in order to determine compliance with design and production standards.

Apparatus

- Balance or scale: Capacity sufficient for the sample mass, accurate to 0.1 percent of the sample mass or readable to 0.1 g and conform to AASHTO M 231
- Sieves, conforming to AASHTO M 92
- Mechanical sieve shaker
- Suitable drying equipment (see FOP for AASHTO T 255)
- Containers and utensils: A pan or vessel of a size sufficient to contain the sample covered with water and to permit vigorous agitation without loss of any part of the sample or water

Sample Sieving

In all procedures it is required to shake the sample over nested sieves. Sieves are selected to furnish information required by specification. The sieves are nested in order of decreasing size from the top to the bottom and the sample, or a portion of the sample, is placed on the top sieve.

Sieves are shaken in a mechanical shaker for approximately 10 minutes, or the minimum time determined to provide complete separation for the sieve shaker being used.

Time Evaluation

The minimum time requirement should be evaluated for each shaker at least annually by the following method: Continue shaking for a sufficient period and in such a manner that, after completion, not more than 0.5 percent by mass of the total sample passes any sieve during one minute of continuous hand sieving.

Provide a snug-fitting pan and cover, and hold in a slightly inclined position in one hand. Strike the side of the sieve sharply and with an upward motion against the heel of the other hand at the rate of about 150 times per minute, turning the sieve about one-sixth of a revolution at intervals of about 25 strokes. In determining sufficiency of sieving for sizes larger than 4.75 mm (No. 4), limit the material on the sieve to a single layer of particles.

Overload Determination

Additional sieves may be necessary to keep from overloading the specified sieves. The sample may also be sieved in increments. For sieves with openings smaller than 4.75 mm (No. 4), the mass retained on any sieve shall not exceed 6 kg/m² (4 g/in²) of sieving surface. For sieves with openings 4.75 mm (No. 4) and larger, the mass (in g) shall not exceed the product of 2500 x (sieve opening in mm) x (effective sieving area in m²). See Table 1.

TABLE 1
Maximum Allowable Mass of Material Retained on a Sieve, g
Nominal Sieve Size, mm (in.)
Exact size is smaller (see AASHTO T 27)

Sieve Size mm (in.)		203 ϕ (8)	305 ϕ (12)	305 x 305 (12 x 12)	350 x 350 (14 x 14)	372 x 580 (16 x 24)
		Sieving Area m ²				
		0.0285	0.0670	0.0929	0.1225	0.2158
90	(3 1/2)	*	15,100	20,900	27,600	48,500
75	(3)	*	12,600	17,400	23,000	40,500
63	(2 1/2)	*	10,600	14,600	19,300	34,000
50	(2)	3600	8400	11,600	15,300	27,000
37.5	(1 1/2)	2700	6300	8700	11,500	20,200
25.0	(1)	1800	4200	5800	7700	13,500
19.0	(3/4)	1400	3200	4400	5800	10,200
16.0	(5/8)	1100	2700	3700	4900	8600
12.5	(1/2)	890	2100	2900	3800	6700
9.5	(3/8)	670	1600	2200	2900	5100
6.3	(1/4)	440	1100	1500	1900	3400
4.75	(No. 4)	330	800	1100	1500	2600
-4.75	(-No. 4)	170	400	560	740	1300

Procedure

1. Using the aggregate sample obtained from the FOP for AASHTO T 308, determine and record the mass of the sample to 0.1 g. This mass shall agree with the mass of the aggregate remaining after ignition (M_f from T 308) within 0.1%.
2. Nest a sieve, such as a 2.0 mm (No. 10), above the 75 μ m (No. 200) sieve.
3. Place the test sample in a container and add sufficient water to cover it. Add a detergent, dispersing agent, or other wetting solution to the water to assure a thorough separation of the material finer than the 75 μ m (No. 200) sieve from the coarser particles. There should be enough wetting agent to produce a small amount of suds when the sample is agitated. Excessive suds may overflow the sieves and carry material away with them.

Note 1: The use of a mechanical apparatus to perform the washing operation is not precluded. Some mechanical washing equipment with some samples may cause degradation of the sample. When mechanical washing equipment is used, the introduction of water, agitating, and decanting may be a continuous operation. Use care not to overflow or overload the 75 μ m (No. 200) sieve.

4. Agitate vigorously to ensure complete separation of the material finer than 75 μ m (No. 200) from coarser particles and bring the fine material into suspension above the coarser material.
5. Immediately pour the wash water containing the suspended and dissolved solids over the nested sieves, being careful not to pour out the coarser particles.
6. Add a second change of water to the sample remaining in the container, agitate, and repeat Step 5. Repeat the operation until the wash water is reasonably clear. Continue washing until the agent is removed.
7. Rinse the material on the nested sieves until water passing through the sieve is reasonably clear.
8. Remove the upper sieve and rinse the material retained on the 0.75 mm (No. 200) sieve until water passing through the sieve is reasonably clear.
9. Return all material retained on the nested sieves to the washed sample by flushing with water.
10. Dry the washed aggregate to constant mass in accordance with the FOP for AASHTO T 255, and then cool prior to sieving. Record the “dry mass after washing”.
11. Select sieves to furnish information required by the specifications. Nest the sieves in order of decreasing size from top to bottom and place the sample, or a portion of the sample, on the top sieve.
12. Place sieves in mechanical shaker and shake for the minimum time determined to provide complete separation for the sieve shaker being used (approximately 10 minutes).

Note 2: Excessive shaking (more than 10 minutes) may result in degradation of the sample.

13. Determine the mass retained on each sieve (individual/cumulative) to the nearest 0.1 g. Ensure that all material trapped in the openings of the sieves are cleaned out and included in the mass retained.

Note 3: Use coarse wire brushes to clean the 600 μ m (No. 30) and larger sieves, and soft bristle brushes for smaller sieves.

Calculation

1. The total mass of the material after sieving should check closely with the original mass of sample placed on the sieves (dry mass after washing). When the masses before and after sieving differ by more than 0.2 percent, do not use the results for acceptance purposes.
2. Divide the masses for each sieve (individual/cumulative) by the total dry mass before washing and multiply by 100 to determine the percent retained on and passing each sieve. Calculate the percent retained and passing each sieve to the nearest 0.1%.
3. Apply the Aggregate Correction Factor to the calculated percent passing, as required in the FOP for AASHTO T 308 “Correction Factors” Steps 11 through 13, to obtain the reported percent passing. Report percentages to the nearest 1% except for the percent passing the 75 μ m (No. 200) sieve, which shall be reported to the nearest 0.1%.

PERCENT RETAINED:

Where:

IPR= Individual Percent Retained

CPR= Cumulative Percent Retained

M= Total Dry Sample mass before washing

IMR= Individual Mass Retained

CMR= Cumulative Mass Retained

$$\text{IPR} = \frac{\text{IMR}}{\text{M}} \times 100 \quad \text{OR} \quad \text{CPR} = \frac{\text{CMR}}{\text{M}} \times 100$$

PERCENT PASSING and REPORTED PERCENT PASSING:

Where:

PP= Calculated Percent Passing

PCP= Previous Calculated Percent Passing

RPP= Reported Percent Passing

$$\text{PP} = \text{PCP} - \text{IPR} \quad \text{OR} \quad \text{PP} = 100 - \text{CPR}$$

$$\text{RPP} = \text{PP} + \text{Aggregate Correction Factor}$$

Report

Results shall be reported on standard forms approved for use by the agency. Depending on the agency, this may include:

- Mass retained on each sieve
- Percent retained on each sieve
- Cumulative mass retained on each sieve
- Cumulative percent retained on each sieve
- Calculated percent passing each sieve to 0.1%
- Aggregate Correction Factor for each sieve from AASHTO T 308
- Reported percent passing

Report percentages to the nearest 1 percent except for the percent passing the 75 μm (No. 200) sieve, which shall be reported to the nearest 0.1 percent.

Addendum WAQTC FOP for AASHTO T 30

Following are guidelines for the use of WAQTC FOP for AASHTO T 30 by the State of Alaska DOT&PF.

1. Calculate the minus 0.075 mm (No. 200) by dividing the sum of the loss from washing plus the mass of the material in the pan by the initial sample weight.
2. If the percent difference between M_f and M exceeds 0.1%, neither the asphalt binder content from WAQTC FOP for AASHTO T 308 nor the sieve analysis shall be used for acceptance. A new portion of the sample shall be tested for Acceptance for both asphalt binder content and gradation in accordance with WAQTC FOPs for AASHTO T 308 and T 30.
3. Calculate the percent difference between M (T 30) and M_f (T 308) according to the following formula:

$$\% \text{ Difference} = \frac{|M_f - M|}{M_f} \times 100$$

This page intentionally left blank

THEORETICAL MAXIMUM SPECIFIC GRAVITY AND DENSITY OF HOT MIX ASPHALT (HMA) (See Addendum for DOT&PF Guidelines) **FOP FOR AASHTO T 209**

Scope

This procedure covers the determination of the maximum specific gravity (G_{mm}) of uncompacted hot mix asphalt (HMA) paving mixtures in accordance with AASHTO T 209. Two methods using two different containers – bowl and flask – are covered.

Specimens prepared in the laboratory shall be cured according to agency standards.

Apparatus

- Balance or scale: Minimum 10,000 g capacity, readable to 0.1 g conforming to AASHTO M 231
- Container: A glass, metal, or plastic bowl or volumetric flask capable of holding a 2,000 g sample and withstanding a partial vacuum
- Container cover: A glass plate or a metal or plastic cover with a vented opening
- Vacuum lid: A transparent lid with a suitable vacuum connection, with a vacuum opening to be covered with a fine wire mesh
- Vacuum pump or water aspirator: Capable of evacuating air from the container to a residual pressure of 4.0 kPa (30 mm Hg)
- Residual pressure manometer or vacuum gauge: Traceable to NIST and capable of measuring residual pressure down to 4.0 kPa (30 mm Hg) or less
- Manometer or vacuum gauge: Capable of measuring the vacuum being applied at the source of the vacuum
- Water bath: A constant-temperature water bath (optional)
- Thermometers: Standardized liquid-in-glass, or electronic digital total immersion type, accurate to 0.5°C (0.9°F)
- Bleeder valve to adjust vacuum
- Timer

Standardization of Flask

Use a volumetric flask that is standardized to accurately determine the mass of water, at $25 \pm 0.5^\circ\text{C}$ ($77 \pm 0.9^\circ\text{F}$), in the flask. The volumetric flask shall be standardized periodically in conformance with procedures established by the agency.

Test Sample Preparation

1. Obtain samples in accordance with the FOP for AASHTO T 168 and reduce according to the FOP for AASHTO R 47.
2. Test sample size shall conform to the requirements of Table 1. Samples larger than the capacity of the container may be tested in two or more increments. Results will be combined and averaged. If the increments have a specific gravity difference greater than 0.018 for the bowl method and 0.011 for the flask method, the test must be re-run.

Table 1
Test Sample Size for G_{mm}

Nominal Maximum Aggregate Size mm (in.)	Minimum Mass g
37.5 or greater (1 ½)	4000
19 to 25 (¾-1)	2500
12.5 or smaller (½)	1500

Procedure – General

Two procedures – bowl and flask – are covered. The first 11 steps are the same for both.

1. Separate the particles of the sample, taking care not to fracture the mineral particles, so that the particles of the fine aggregate portion are not larger than 6.3 mm (¼ in.). If the mixture is not sufficiently soft to be separated manually, place it in a large flat pan and warm in an oven only until it is pliable enough for separation.
2. Cool the sample to room temperature.
3. Determine and record the mass of the dry bowl or flask, including the cover, to the nearest 0.1 g.
4. Place the sample in the bowl or flask.
5. Determine and record the mass of the dry bowl or flask, cover, and sample to the nearest 0.1 g.
6. Determine and record the mass of the sample by subtracting the mass determined in Step 3 from the mass determined in Step 5. Designate this mass as “A”.
7. Add sufficient water at approximately 25° ±1°C (77° ±1.8°F) to cover the sample by about 25 mm (1 in.).

Note 1: The release of entrapped air may be facilitated by the addition of a wetting agent. Check with the agency to see if this is permitted and, if it is, for a recommended agent.

8. Place the lid on the bowl or flask and attach the vacuum line. To ensure a proper seal between the flask and the lid, wet the O-ring or use a petroleum gel.
9. Remove entrapped air by subjecting the contents to a partial vacuum of 3.7 ±0.3 kPa (27.5 ±2.5 mm Hg) residual pressure for 15 ±2 minutes.
10. Agitate the container and contents, either continuously by mechanical device or manually by vigorous shaking, at 2 minute intervals. This agitation facilitates the removal of air.

11. Turn off the vacuum pump, slowly open the release valve, and remove the lid. When performing the flask method, complete steps 12B through 16B within 10 ± 1 minutes.

Procedure – Bowl

- 12A. Suspend and immerse the bowl and contents in water at $25 \pm 1.0^{\circ}\text{C}$ ($77 \pm 1.8^{\circ}\text{F}$) for 10 ± 1 minutes. The holder shall be immersed sufficiently to cover both it and the bowl.
- 13A. Determine and record the submerged weight of the bowl and contents to the nearest 0.1 g.
- 14A. Empty and re-submerge the bowl following Step 12A to determine the submerged weight of the bowl to the nearest 0.1 g.
- 15A. Determine and record the submerged weight of the sample the nearest 0.1 g by subtracting the submerged weight of the bowl from the submerged weight determined in Step 13A. Designate this submerged weight as “C”.

Procedure – Flask

- 12B. Immediately fill the flask with water without reintroducing air.
- 13B. Stabilize the temperature of the flask and contents in a water bath so that the final temperature is within $25 \pm 1^{\circ}\text{C}$ ($77 \pm 1.8^{\circ}\text{F}$).
Note 2: In lieu of placing the flask in the water bath, determine the temperature of the water in the flask and make the appropriate density correction using Table 2 when the temperature is outside $25 \pm 1^{\circ}\text{C}$ ($77 \pm 1.8^{\circ}\text{F}$).
- 14B. Finish filling the flask, place the cover or a glass plate on the flask, and eliminate all air from the flask.
Note 3: When using the metal flask and cover, place the cover on the flask and push down slowly, forcing excess water out of the hole in the center of the cover. Use care when filling flask to avoid reintroducing air into the water.
- 15B. Towel dry the outside of the flask and cover.
- 16B. Determine and record the mass of the flask, cover, de-aired water, and sample to the nearest 0.1 g within 10 ± 1 minutes of completion of Step 11. Designate this mass as “E”.

Procedure – Mixtures Containing Uncoated Porous Aggregate

If the pores of the aggregates are not thoroughly sealed by a bituminous film, they may become saturated with water during the vacuuming procedure, resulting in an error in maximum density. To determine if this has occurred, complete the general procedure and then:

1. Carefully drain water from sample through a towel held over the top of the container to prevent loss of material.
2. Spread sample before an electric fan to remove surface moisture.
3. Determine the mass of the sample when the surface moisture appears to be gone.
4. Continue drying and determine the mass of the sample at 15-minute intervals until less than a 0.5 g loss is found between determinations.

5. Record the mass as the saturated surface dry mass to the nearest 0.1 g. Designate this mass as “A_{SSD}”.
6. Calculate, as indicated below, G_{mm}, using “A” and “A_{SSD}”, and compare the two values.

Calculation

Calculate the G_{mm} to three decimal places as follows:

Bowl Procedure

$$G_{mm} = \frac{A}{A - C}$$

where:

A = mass of dry sample in air, g

C = submerged weight of sample in water, g

Flask Procedure

$$G_{mm} = \frac{A}{A + D - E} \times R \quad \text{or} \quad G_{mm} = \frac{A}{A_{SSD} + D - E} \times R$$

where: (for mixtures containing uncoated aggregate materials)

A = Mass of dry sample in air, g

A_{SSD} = Mass of saturated surface-dry sample in air, g

D = Mass of flask filled with water at 25°C (77°F), g, determined during the Standardization of Flask procedure

E = Mass of flask filled with water and the test sample at test temperature, g

R = Factor from Table 2 to correct the density of water – use when a test temperature is outside 25 ± 1°C (77 ± 1.8°F)

Average

$$2.470 - 2.466 = 0.004 \quad 0.004 \div 2 = 0.002 \quad 0.002 + 2.466 = \mathbf{2.468}$$

$$\text{Or } 2.470 + 2.466 = 4.936 \quad 4.936 \div 2 = 2.468$$

Table 2
Temperature Correction Factor

°C	°F	“R”		°C	°F	“R”
20.0	68.0	1.00117		23.3	74.9	1.00042
20.1	68.2	1.00114		23.4	74.1	1.00040
20.2	68.4	1.00112		23.5	74.3	1.00037
20.3	68.5	1.00110		23.6	74.5	1.00035
20.4	68.7	1.00108		23.7	74.7	1.00033
20.5	68.9	1.00106		23.8	74.8	1.00030
20.6	69.1	1.00104		23.9	75.0	1.00028
20.7	69.3	1.00102		24.0	75.2	1.00025
20.8	69.4	1.00100		24.1	75.4	1.00023
20.9	69.6	1.00097		24.2	75.6	1.00020
21.0	69.8	1.00095		24.3	75.7	1.00018
21.1	70.0	1.00093		24.4	75.9	1.00015
21.2	70.2	1.00091		24.5	76.1	1.00013
21.3	70.3	1.00089		24.6	76.3	1.00010
21.4	70.5	1.00086		24.7	76.5	1.00007
21.5	70.7	1.00084		24.8	76.6	1.00005
21.6	70.9	1.00082		24.9	76.8	1.00002
21.7	71.1	1.00080		25.0	77.0	1.00000
21.8	71.2	1.00077		25.1	77.2	0.99997
21.9	71.4	1.00075		25.2	77.4	0.99995
22.0	71.6	1.00073		25.3	77.5	0.99992
22.1	71.8	1.00030		25.4	77.7	0.99989
22.2	72.0	1.00068		25.5	77.9	0.99987
22.3	72.1	1.00066		25.6	78.1	0.99984
22.4	72.3	1.00064		25.7	78.3	0.99981
22.5	72.5	1.00061		25.8	78.4	0.99979
22.6	72.7	1.00059		25.9	78.6	0.99976
22.7	72.9	1.00057		26.0	78.8	0.99973
22.8	73.0	1.00054		26.1	79.0	0.99971
22.9	73.2	1.00052		26.2	79.2	0.99968
23.0	73.4	1.00050		26.3	79.3	0.99965
23.1	73.6	1.00047		26.4	79.5	0.99963
23.2	73.8	1.00045		26.5	79.7	0.99960

Theoretical Maximum Density

To calculate the theoretical maximum density at 25°C (77°F) use one of the following formulas. The density of water at 25°C (77°F) is 997.1 in Metric units or 62.245 in English units.

Theoretical maximum density $\text{kg/m}^3 = G_{\text{mm}} \times 997.1 \text{ kg/m}^3$

or

Theoretical maximum density $\text{lb/ft}^3 = G_{\text{mm}} \times 62.245 \text{ lb/ft}^3$

Report

Results shall be reported on standard forms approved for use by the agency. Report G_{mm} to three decimal places. Report the theoretical maximum density to 1 kg/m^3 (0.1 lb/ft^3).

Addendum WAQTC FOP for AASHTO T 209

Following are guidelines for the use of WAQTC FOP for AASHTO T 209 by the State of Alaska DOT&PF.

1. The flask method is to be used in all Theoretical Maximum Specific Gravity determinations.
2. Replace Table 1 to the following:

Table 1
Test Sample Size for Maximum Specific Gravity

Nominal Maximum Aggregate Size* mm (in.)	Minimum Mass g
25 (1)	2500
19 (3/4)	2000
12.5 (1/2)	1500
9.5 (3/8)	1000
4.75 (No. 4)	0500

This page intentionally left blank.

BULK SPECIFIC GRAVITY OF COMPACTED HOT MIX ASPHALT (HMA) USING SATURATED SURFACE-DRY SPECIMENS (See Addendum for DOT&PF Guidelines) **FOP FOR AASHTO T 166**

BULK SPECIFIC GRAVITY OF COMPACTED HOT MIX ASPHALT (HMA) USING PARAFFIN-COATED SPECIMENS **FOP FOR AASHTO T 275**

Scope

This procedure covers the determination of bulk specific gravity (G_{mb}) of compacted hot mix asphalt (HMA) using three methods – A, B, and C – in accordance with AASHTO T 166. These three methods are for use on specimens not having open or interconnecting voids and/or absorbing more than 2.0 percent water by volume. A fourth and fifth method – D & E – in accordance with AASHTO T 275 and covering specimens having open or interconnecting voids and/or absorbing more than 2.0 percent water by volume is also included.

Overview

- Method A: Suspension
- Method B: Volumeter
- Method C: Rapid test for A or B

- Method D: Suspension for coated specimen
- Method E: Volumeter for coated specimen

Test Specimens

Test specimens may be either laboratory-molded or from HMA pavement. For specimens it is recommended that the diameter be equal to four times the maximum size of the aggregate and the thickness be at least one and one half times the maximum size.

Terminology

Constant Mass: AASHTO T 166 defines constant mass as the mass at which further drying at $52 \pm 3^{\circ}\text{C}$ ($125 \pm 5^{\circ}\text{F}$) does not alter the mass by more than 0.05 percent. It also states that samples shall initially be dried overnight and that mass determinations shall be made at 2-hour drying intervals. AASHTO T 166 also states that recently molded laboratory samples that have not been exposed to moisture do not need drying.

Apparatus - Method A (Suspension)

- Balance or scale: 5 kg capacity, readable to 0.1 g, and fitted with a suitable suspension apparatus and holder to permit weighing the specimen while suspended in water, conforming to AASHTO M 231.
- Suspension apparatus: Wire of the smallest practical size and constructed to permit the container to be fully immersed.

- Water bath: For immersing the specimen in water while suspended under the balance or scale, and equipped with an overflow outlet for maintaining a constant water level.
- Towel: Damp cloth towel used for surface drying specimens.
- Oven: Capable of maintaining a temperature of $110 \pm 5^{\circ}\text{C}$ ($230 \pm 9^{\circ}\text{F}$) for drying the specimens to a constant mass.
- Pan: Pan or other suitable container of known mass, large enough to hold a sample for drying in oven.
- Thermometer: Having a range of 19 to 27°C (66 to 80°F), graduated in 0.1°C (0.2°F) subdivisions.

Procedure - Method A (Suspension)

1. Dry the specimen to constant mass, if required.

Note 1: To expedite the procedure, steps 1 and 2 may be performed last. To further expedite the process, see Method C.

2. Cool the specimen in air to $25 \pm 5^{\circ}\text{C}$ ($77 \pm 9^{\circ}\text{F}$), and determine and record the dry mass to the nearest 0.1 g. Designate this mass as “A”.
3. Fill the water bath to overflow level with water at $25 \pm 1^{\circ}\text{C}$ ($77 \pm 1.8^{\circ}\text{F}$) and allow the water to stabilize.
4. Zero or tare the balance with the immersion apparatus attached, ensuring that the device is not touching the sides or the bottom of the water bath.
5. Immerse the specimen for 4 ± 1 minutes.
6. Determine and record the submerged weight to the nearest 0.1 g. Designate this submerged weight as “C”.
7. Steps 7 through 9 must be completed within 5 seconds. Remove the sample from the water and quickly surface dry with a damp cloth towel.
8. Zero or tare the balance.
9. Determine and record the mass of the SSD specimen to nearest 0.1 g. Designate this mass as “B”. Any water that seeps from the specimen during the mass determination is considered part of the saturated specimen.

Calculations - Method A (Suspension)

$$G_{mb} = \frac{A}{B - C}$$

where:

A = Mass of dry specimen in air, g

B = Mass of SSD specimen in air, g

C = Weight of specimen in water at $25 \pm 1^{\circ}\text{C}$ ($77 \pm 1.8^{\circ}\text{F}$), g

$$\text{Percent Water Absorbed (by volume)} = \frac{B - A}{B - C} \times 100$$

Apparatus - Method B (Volumeter)

- Balance or scale: 5 kg capacity, readable to 0.1 g and conforming to AASHTO M 231.
- Water bath: Thermostatically controlled to $25 \pm 0.5^{\circ}\text{C}$ ($77 \pm 0.9^{\circ}\text{F}$).
- Thermometer: Range of 19 to 27°C (66 to 80°F), and graduated in 0.1°C (0.2°F) subdivisions.
- Volumeter: Calibrated to 1200 mL or appropriate capacity for test sample and having a tapered lid with a capillary bore.
- Oven: Capable of maintaining a temperature of $110 \pm 5^{\circ}\text{C}$ ($230 \pm 9^{\circ}\text{F}$) for drying the specimens to a constant mass.
- Pan: Pan or other suitable container of known mass, large enough to hold a sample for drying in oven.
- Towel: Damp cloth towel used for surface drying specimens.

Procedure - Method B (Volumeter)

1. Dry the specimen to constant mass, if required.

Note 1: To expedite the procedure, steps 1 and 2 may be performed last. To further expedite the process, see Method C.

2. Cool the specimen in air to $25 \pm 5^{\circ}\text{C}$ ($77 \pm 9^{\circ}\text{F}$), and determine and record the dry mass to the nearest 0.1 g. Designate this mass as “A”.
3. Immerse the specimen in the temperature-controlled water bath for at least 10 minutes.
4. Fill the volumeter with distilled water at $25 \pm 1^{\circ}\text{C}$ ($77 \pm 1.8^{\circ}\text{F}$) making sure some water escapes through the capillary bore of the tapered lid. Wipe the volumeter dry. Determine the mass of the volumeter to the nearest 0.1 g. Designate this mass as “D”.
5. Steps 5 and 6 must be completed within 5 seconds. At the end of the ten minute period, remove the specimen from the water bath and quickly surface dry with a damp cloth towel.
6. Determine and record the mass of the SSD specimen to the nearest 0.1 g. Designate this mass as “B”. Any water that seeps from the specimen during the mass determination is considered part of the saturated specimen.
7. Place the specimen in the volumeter and let stand 60 seconds.
8. Bring the temperature of the water to $25 \pm 1^{\circ}\text{C}$ ($77 \pm 1.8^{\circ}\text{F}$) and cover the volumeter, making sure some water escapes through the capillary bore of the tapered lid.
9. Wipe the volumeter dry.
10. Determine and record the mass of the volumeter and specimen to the nearest 0.1 g. Designate this mass as “E”.

Note 2: Method B is not acceptable for use with specimens that have more than 6% air voids.

Calculations - Method B (Volumeter)

$$G_{mb} = \frac{A}{B + D - E}$$

where:

A = Mass of dry specimen in air, g

B = Mass of SSD specimen in air, g

D = Mass of volumeter filled with water at $25 \pm 1^\circ\text{C}$ ($77 \pm 1.8^\circ\text{F}$), g

E = Mass of volumeter filled with specimen and water, g

$$\text{Percent Water Absorbed (by volume)} = \frac{B - A}{B + D - E} \times 100$$

Apparatus - Method C (Rapid Test for Method A or B)

See Methods A or B.

Note 3: This procedure can be used for specimens that are not required to be saved and contain substantial amounts of moisture. Cores can be tested the same day as obtained by this method.

Procedure - Method C (Rapid Test for Method A or B)

1. Determine which method to perform, A or B. Proceed with Method A or B, except that the dry mass, A, is determined last. In method A and B, start on Step 3 and complete that procedure, then continue as follows to determine mass "A".
2. Place the specimen on a large, flat-bottom pan of known mass.
3. Heat at a minimum of 105°C (221°F), until the specimen can be easily separated to the point where the fine aggregate particles are not larger than 6.3 mm (1/4 in.). In no case should the Job Mix Formula mixing temperature be exceeded.
4. Dry to constant mass. Constant mass is defined as the mass at which further drying at the temperature in Step 3 does not change by more than 0.05% after an additional 2 hour drying time.
5. Cool in air to $25 \pm 5^\circ\text{C}$ ($77 \pm 9^\circ\text{F}$).
6. Determine and record the mass of the pan and specimen to the nearest 0.1 g.
7. Determine and record the mass of the dry specimen to the nearest 0.1 g by subtracting the mass of the pan from the mass determined in Step 6. Designate this mass as "A".

Calculations - Method C (Rapid Test for Method A or B)

Complete the calculations as outlined in Methods A or B, as appropriate.

Materials - Method D Suspension (Coated Specimens/AASHTO T 275)

- Paraffin or parafilm: Used to coat test specimens.

Apparatus - Method D Suspension (Coated Specimens/AASHTO T 275)

- Balance or scale: 5 kg capacity, readable to 0.1 g, and fitted with a suitable suspension apparatus and holder to permit weighing the specimen while suspended in water, conforming to AASHTO M 231.
- Suspension apparatus: Wire of the smallest practical size and constructed to permit the container to be fully immersed.
- Water bath: For immersing the specimen in water while suspended under the balance or scale, and equipped with an overflow outlet for maintaining a constant water level.
- Oven: Capable of maintaining a temperature of $110 \pm 5^{\circ}\text{C}$ ($230 \pm 9^{\circ}\text{F}$) for drying the specimens to a constant mass.
- Pan: Pan or other suitable container of known mass, large enough to hold a sample for drying in oven.

Procedure - Method D Suspension (Coated Specimens/AASHTO T 275)

1. Dry the specimen to constant mass, if required2. Cool the specimen in air to $25 \pm 5^{\circ}\text{C}$ ($77 \pm 9^{\circ}\text{F}$), and determine and record the dry mass to the nearest 0.1 g. Designate this mass as “A”.
3. Coat the specimen on all surfaces with melted paraffin, or parafilm coating, sufficiently thick to seal all voids.
4. Allow coating to cool in air at $25 \pm 5^{\circ}\text{C}$ ($77 \pm 9^{\circ}\text{F}$) for 30 minutes.
5. Determine and record the mass of the coated specimen to the nearest 0.1 g. Designate this mass as “D”.
6. Fill the water bath to overflow level with water at $25 \pm 1^{\circ}\text{C}$ ($77 \pm 1.8^{\circ}\text{F}$).
7. Immerse the specimen in water at $25 \pm 1^{\circ}\text{C}$ ($77 \pm 1.8^{\circ}\text{F}$) for 4 ± 1 minutes.
8. Determine and record the submerged weight to the nearest 0.1 g. Designate this submerged weight as “E”.
9. Determine the specific gravity of paraffin or parafilm at $25 \pm 1^{\circ}\text{C}$ ($77 \pm 1.8^{\circ}\text{F}$) from the manufacturer’s literature or other suitable source. Designate this specific gravity as “F”.

Calculations - Method D Suspension (Coated Specimens/AASHTO T 275)

$$G_{mb} = \frac{A}{D - E - \left[\frac{D - A}{F} \right]}$$

where:

A = Mass of dry specimen in air, g

D = Mass of specimen with paraffin coating in air, g

E = Weight of specimen with paraffin coating in water, g

F = Specific gravity of paraffin or parafilm at $25 \pm 1^\circ\text{C}$ ($77 \pm 1.8^\circ\text{F}$)

Apparatus - Method E Volumeter (Coated Specimens/AASHTO T 275)

- Balance or scale: 5 kg capacity, readable to 0.1 g and conforming to AASHTO M 231.
- Water bath: Thermostatically controlled to $25 \pm 0.5^\circ\text{C}$ ($77 \pm 0.9^\circ\text{F}$).
- Thermometer: Range of 19 to 27°C (66 to 80°F), and graduated in 0.1°C (0.2°F) subdivisions.
- Volumeter: Calibrated to 1200 mL or appropriate capacity for test sample and having a tapered lid with a capillary bore.
- Oven: Capable of maintaining a temperature of $110 \pm 5^\circ\text{C}$ ($230 \pm 9^\circ\text{F}$) for drying the specimens to a constant mass.
- Pan: Pan or other suitable container of known mass, large enough to hold a sample for drying in oven.
- Towel: Damp cloth towel used for surface drying specimens.

Procedure - Method E Volumeter (Coated Specimens/AASHTO T 275)

1. Dry the specimen to constant mass, if required.
2. Cool the specimen in air to $25 \pm 5^\circ\text{C}$ ($77 \pm 9^\circ\text{F}$), and determine and record the dry mass to the nearest 0.1 g. Designate this mass as "A".
3. Coat the specimen on all surfaces with paraffin, or parafilm coating, sufficiently thick to seal all voids.
4. Allow coating to cool in air at $25 \pm 5^\circ\text{C}$ ($77 \pm 9^\circ\text{F}$) for 30 minutes.
5. Determine and record the mass of the coated specimen to the nearest 0.1g. Designate this mass as "C".
6. Fill the volumeter with distilled water at $25 \pm 1^\circ\text{C}$ ($77 \pm 1.8^\circ\text{F}$) and place the coated specimen in the volumeter.
7. Bring the temperature of the water to $25 \pm 1^\circ\text{C}$ ($77 \pm 1.8^\circ\text{F}$) and cover the volumeter, making sure some water escapes through the capillary bore of the tapered lid.

8. Wipe the volumeter dry.
9. Determine and record the mass of the volumeter and specimen to the nearest 0.1 g. Designate this mass as “E”.
10. Determine the specific gravity of paraffin or parafilm at $25 \pm 1^\circ\text{C}$ ($77 \pm 1.8^\circ\text{F}$) or from the manufacturer’s literature or other suitable source. Designate this specific gravity as “F”.

Calculations - Method E Volumeter (Coated Specimens/AASHTO T 275)

$$G_{mb} = \frac{A}{D - \left[E - C + \left(\frac{C - A}{F} \right) \right]}$$

where:

A = Mass of dry specimen in air, g

C = Mass of specimen with paraffin coating in air, g

D = Mass of volumeter filled water at $25 \pm 1^\circ\text{C}$ ($77 \pm 1.8^\circ\text{F}$), g

E = Mass of volumeter filled with specimen with paraffin coating and in water at $25 \pm 1^\circ\text{C}$ ($77 \pm 1.8^\circ\text{F}$), g

F = Specific gravity of paraffin or parafilm at $25 \pm 1^\circ\text{C}$ ($77 \pm 1.8^\circ\text{F}$)

Report

Results shall be reported on standard forms approved for use by the agency. Report the G_{mb} to 3 decimal places and absorption to 2 decimal places. Report the method performed.

Addendum WAQTC FOP for AASHTO T 166/T 275

Following are guidelines for the use of WAQTC FOP for AASHTO T 166/T 275 by the State of Alaska DOT&PF.

1. Report compaction to the 0.1%. Calculate as follows:

$$C_p = \left(\frac{G_{mb}}{G_{mm}} \right) \times 100$$

Where:

C_p = Percent Compaction

G_{mm} = Theoretical Maximum Specific Gravity

G_{mb} = Bulk Specific Gravity

2. Method C/A is the only accepted method for AKDOT&PF projects, regardless of the absorption calculated.
3. As an alternate to drying to constant mass in an oven, ASTM D 7227 may be used.

IN-PLACE DENSITY OF BITUMINOUS MIXES USING THE NUCLEAR MOISTURE-DENSITY GAUGE (See Addendum for DOT&PF Guidelines)

FOP FOR WAQTC TM 8

Scope

This test method describes a test procedure for determining the density of bituminous mixes by means of a nuclear gauge employing either direct transmission or backscatter methods. Correlation with densities determined under the FOP for AASHTO T 166 is required by some agencies.

Apparatus

- Nuclear density gauge with the factory-matched standard reference block.
- Drive pin, guide/scrapper plate, and hammer for testing in direct transmission mode.
- Transport case for properly shipping and housing the gauge and tools.
- Instruction manual for the specific make and model of gauge.
- Radioactive materials information and calibration packet containing:
 - Daily standard count log
 - Factory and laboratory calibration data sheet
 - Leak test certificate
 - Shippers' declaration for dangerous goods
 - Procedure memo for storing, transporting and handling nuclear testing equipment
 - Other radioactive materials documentation as required by local regulatory requirements

Material

- Filler material: Fine-graded sand from the source used to produce the asphalt pavement or other agency approved materials.

Radiation Safety

This method does not purport to address all of the safety problems associated with its use. This test method involves potentially hazardous materials. The gauge utilizes radioactive materials that may be hazardous to the health of the user unless proper precautions are taken. Users of this gauge must become familiar with the applicable safety procedures and governmental regulations. All operators will be trained in radiation safety prior to operating nuclear density gauges. Some agencies require the use of personal monitoring devices such as a thermoluminescent dosimeter or film badge. Effective instructions, together with routine safety procedures such as source leak tests, recording and evaluation of personal monitoring device data, etc., are a recommended part of the operation and storage of this gauge.

Calibration

Calibrate the nuclear gauge as required by the agency. This calibration may be performed by the agency using the manufacturer's recommended procedures or by other facilities approved by the agency. Verify or re-establish calibration curves, tables, or equivalent coefficients every 12 months.

Standardization

1. Turn the gauge on and allow it to stabilize (approximately 10 to 20 minutes) prior to standardization. Leave the power on during the day's testing.
2. Standardize the nuclear gauge at the construction site at the start of each day's work and as often as deemed necessary by the operator or agency. Daily variations in standard count shall not exceed the daily variations established by the manufacturer of the gauge. If the daily variations are exceeded after repeating the standardization procedure, the gauge should be repaired and/or recalibrated.
3. Record the standard count for both density and moisture in the daily standard count log. The exact procedure for standard count is listed in the manufacturer's Operator's Manual.

Note 1: New standard counts may be necessary more than once a day. See agency requirements.

Test Site Location

1. Select a test location(s) randomly and in accordance with agency requirements. Test sites should be relatively smooth and flat and meet the following conditions:
 - a. At least 10 m (30 ft) away from other sources of radioactivity.
 - b. At least 3 m (10 ft) away from large objects.
 - c. If the gauge will be closer than 600 mm (24 in.) to any vertical mass, or less than 300 mm (12 in.) from a vertical pavement edge, use the gauge manufacturer's correction procedure.

Overview

There are two methods for determining the in-place density of HMA. See agency requirements for method selection.

- Direct Transmission
- Backscatter

Procedure

Direct Transmission

1. Maximum contact between the base of the gauge and the surface of the material under test is critical.
2. Use the guide and scraper plate as a template and drill a hole to a depth of at least 7 mm (1/4 in.) deeper than the measurement depth required for the gauge.
3. Place the gauge on the prepared surface so the source rod can enter the hole. Insert the probe in the hole and lower the source rod to the desired test depth using the handle and trigger mechanism. Position the gauge with the long axis of the gauge parallel to the direction of paving. Pull the gauge so that the probe is firmly against the side of the hole.
4. Take one four-minute test and record the wet density (WD) reading.

Backscatter

1. Maintain maximum contact between the base of the gauge and the surface of the material under test. Use filler material to fill surface voids. Spread a small amount of filler material over the test site surface and distribute it evenly. Strike off the surface with a straightedge (such as a lathe or flat-bar steel) to remove excess material.
2. Place the gauge on the test site. Using a crayon (not spray paint), mark the outline or footprint of the gauge. Extend the probe to the backscatter position.
3. Take a one-minute test and record the wet density reading.
4. Rotate the gauge 90 degrees about the probe. Mark the outline or footprint of the gauge.
5. Take another one-minute test and record the wet density reading.
6. If the difference between the two one-minute tests is greater than 40 kg/m³ (2.5 lb/ft³), retest in both directions.
7. The density reported for each test site shall be the average of the two individual one-minute wet density readings.

Calculation of Results


Percent compaction is determined by comparing the in-place wet density as determined by this method to the appropriate agency density standard. See appropriate agency policy for use of density standards.

$$\frac{\text{Corrected Reading}}{\text{Maximum Density}} \times 100 = \% \text{ compaction}$$

Correlation with Cores

Note 2: When density correlation with the FOP for AASHTO T 166 is required, correlation of the nuclear gauge with pavement cores shall be made on the first day's paving (within 24 hours) or from a test strip constructed prior to the start of paving. Cores must be taken before traffic is allowed on the pavement.

1. Determine the number of cores required for correlation from the agency's specifications. Cores shall be located on the first day's paving or on the test strip. Locate the test sites in accordance with the agency's specifications. Follow the "Procedure" section above to establish test sites and obtain densities using the nuclear gauge.
2. Obtain a pavement core from each of the test sites in accordance with WAQTC TM 11. The core should be taken from the center of the nuclear gauge footprint. If direct transmission was used, locate the core at least 25 mm (1 in.) away from the edge of the drive pin hole.

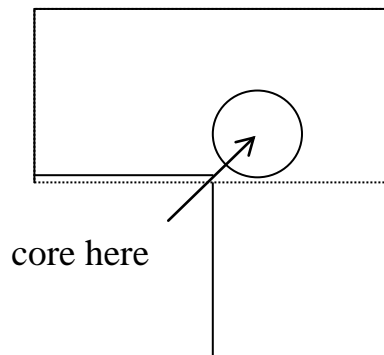

3. Determine the density of the cores by the FOP for AASHTO T 166, Bulk Specific Gravity of Compacted Bituminous Mixtures Using Saturated Surface Dry Specimens.
4. Calculate a correlation factor for the nuclear gauge reading as follows:
 - a. Calculate the difference between the core density and nuclear gauge density at each test site to the nearest 1 kg/m^3 (0.1 lb/ft^3). Calculate the average difference and standard deviation of the differences for the entire data set to the nearest 1 kg/m^3 (0.1 lb/ft^3).
 - b. If the standard deviation of the differences is equal to or less than 40 kg/m^3 (2.5 lb/ft^3), the correlation factor applied to the nuclear density gauge reading shall be the average difference calculated above in 4.a.
 - c. If the standard deviation of the differences is greater than 40 kg/m^3 (2.5 lb/ft^3), the test site with the greatest variation from the average difference shall be eliminated from the data set and the data set properties and correlation factor recalculated following 4.a and 4.b.
 - d. If the standard deviation of the modified data set still exceeds the maximum specified in 4.b, additional test sites will be eliminated from the data set and the data set properties and correlation factor recalculated following 4.a and 4.b. If the data set consists of less than five test sites, additional test sites shall be established.

Note 3: The exact method used in calculating the nuclear gauge correlation factor shall be defined by agency policy.

Note 4: The above correlation procedure must be repeated if there is a new job mix formula. Adjustments to the job mix formula beyond tolerances established in the contract documents will constitute a new job mix formula. A correlation factor established using this procedure is only valid for the particular gauge and in the mode and at the probe depth used in the correlation procedure. If another gauge is brought onto the project, it shall be correlated using the same procedure. Multiple gauges may be correlated from the same series of cores if done at the same time.

Note 5: For the purpose of this procedure, a job mix formula is defined as the percent and grade of paving asphalt used with a specified gradation of aggregate from a designated aggregate source. A new job mix formula may be required whenever compaction of the wearing surface exceeds the agency's specified maximum density or minimum air voids.

Report

Results shall be reported on standard forms approved by the agency. Include the following information:

- Location of test and thickness of layer tested
- Mixture type
- Make, model and serial number of the nuclear moisture-density gauge
- Mode of measurement, depth, calculated wet density of each measurement and any adjustment data
- Standard density
- Percent compaction and/or percent air voids
- Name and signature of operator

Addendum WAQTC TM 8

Following are guidelines for the use of WAQTC TM 8 by the State of Alaska DOT&PF.

1. Testing under this method shall be used for quality control and when specified, acceptance testing.
2. All density testing on HMA done under this method shall be done in Backscatter only.
3. Report percent compaction to the nearest 0.1%

Relative Standard Density by the Control Strip Method ATM 412

1. Scope

This method describes a procedure for determining the relative standard density of a material by the control strip testing method. This is applicable to granular materials that are bound together with asphalt binders and/or portland cement.

2. Significance and Use

In testing some HMA's, determining the standard density may be difficult with conventional test methods used in the laboratory. When these problems occur a method that allows the determination of a relative standard density in the field can facilitate the verification of compaction efforts. This method describes a procedure to determine the relative standard density to be used in these circumstances.

3. Apparatus

- Nuclear Moisture/Density Gauge—Calibrate and standardize in accordance with WAQTC TM 8.
- Compaction equipment that meets the requirements of the contract and of sufficient size and compaction energy to compact the material.

4. Site Preparation

1. The Engineer will designate the location and the size of the control strip, as well as minimum compaction equipment to be used.
2. The subgrade will be compacted to a minimum density equal to that required for the material being tested. When the compaction is complete, the Engineer will approve the surface.
3. A representative lift of the material being evaluated will be placed and prepared for compaction.

5. Procedure

1. Attention should be paid to the requirements of the product being placed so that any binder content, temperature and/or moisture requirements are maintained in an acceptable range.
2. A minimum of 3 test locations will be selected with-in the control strip. The locations will be in the middle 1/2 of the control strip and at least 12 in from the edge of the control strip. The Engineer will select test locations.
3. The locations will be marked in such a way as not to be lost during the compaction of the control strip. This can be accomplished by marking the side of the strip with stakes or surveyors tape, or by marking with paint beside the location on the control strip.
4. Test time (15 second or 1 minute) using 1 reading or average of two will be as approved by the Engineer
5. Care should be taken when preparing the test location so that it is flat and the surface voids filled. If necessary, use a small quantity of dry sand to fill the voids. This layer will in no case be more than 1/8 in in depth.
6. After the first pass with the compaction equipment, an initial density test is taken and recorded.

Note 1: One pass of the roller will be defined as one roll over the location.
7. After each subsequent pass and for each piece of compaction equipment used, a test is taken at each location and recorded.
8. Continue the compaction and testing cycle until either of these conditions is met.

- a. There is less than 1 lb/ft³ increase in the density of the averaged density tests for each location on two consecutive passes.
 - b. There is less than 16 kg/m³ (1 lb/ft³) increase in the density of the average of all three locations for two consecutive passes.
9. Select ten random locations on the completed control strip and test by averaging two one minute counts at each location in accordance with TM 8. Average the results from the ten locations and this value will be the relative standard density for this material.

Note 2: It may be necessary to repeat the procedure for additional roller types depending on the material to be tested and the requirements of sequencing for the finished surface.

10. Additional control strips may be required if there are changes in the material, lift thickness or compaction equipment.

6. Calculations

1. The Relative Standard Density value will be calculated as follows:

$$D_s = \frac{(A_1 + A_2 + A_3 + A_4 + A_5 + A_6 + A_7 + A_8 + A_9 + A_{10})}{10}$$

Where:

D_s = Relative Standard Density for the material.

A_n = Average Density for random test location n .

7. Report

- Report the average density for each pass
- Report the standard density to the nearest 0.1 lb/ft³

SAMPLING BITUMINOUS MATERIAL AFTER COMPACTION (OBTAINING CORES)

WAQTC TM 11 (See Addendum for DOT&PF Guidelines)

Scope

- This method describes the process for removal of a sample of compacted bituminous material from a pavement for laboratory testing by obtaining test cores after compaction has been completed. Core diameter(s) may range in size from 2 in. to 12 in.
- The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only.

Significance And Use

- Samples obtained in accordance with the procedure given in this practice may be used for measuring pavement thickness, density, and acceptance testing.
- When cores are used to determine nuclear gauge correlation, see WAQTC TM 8.
- When cores are used to determine pavement density, the Bulk Specific Gravity (G_{mb}) is determined according to WAQTC FOP for AASHTO T 166 / T 275.

Apparatus

- Coring Machine – To minimize distortion of the compacted bituminous cores, a motor driver core machine shall be used to secure the sample that is capable of obtaining a core the full depth of the bituminous material being placed.
- Core Bit – The cutting edge of the core drill bit shall be of hardened steel or other suitable material with diamond chips embedded in the metal cutting edge.
- Separation Equipment – Cores shall be separated with a saw or other method(s) that provides a clean smooth plane representing the layer to be measured, or tested.
- Retrieval Device – A retrieval device for removing core samples from holes that will preserve the integrity of the core. The device may be a steel rod of suitable length and with a diameter that will fit into the space between the core and the pavement material. There shall be a 90 degree bend at the top to form a handle and a 90 degree bend at the bottom, approximately 50 mm (2 in.) long, forming a hook to assist in the retrieval of the core.

Material

- Water, ice, dry ice, liquid nitrogen, or other cooling material.

Safety

- This method does not purport to address all of the safety problems associated with its use. This test method involves potentially hazardous conditions.

Test Site Location

- The quantity of cores to be obtained shall be determined by the test procedure to be performed or agency requirements.
- Determine the location of the core(s) as required by the agency.

Procedure

- For freshly placed bituminous materials, the core shall be taken when the material has had sufficient amount of time to cool to prevent damage to the core.
- Cores may be taken by cooling the pavement to allow for immediate removal. Cooling may be expedited with the use of water, ice water, ice, or dry ice.
- Place the coring machine and core bit over the selected location.
- Start the flow of coolant to ensure removal of the cuttings and to minimize the generation of heat caused by friction.
- Keep the core bit perpendicular to the bituminous surface during the coring process. If any portion of the coring machine shifts during the operation, the core may break or distort.
- Constant downward pressure should be applied on the core bit. Failure to apply constant pressure, or too much pressure, may cause the bit to bind or distort the core.
- Continue the coring operation until the desired depth is achieved.
- If necessary, use a retrieval device to remove the core.
- If the core is damaged to a point that it can not be utilized for its intended purpose, a new core shall be obtained within 12 in. of the original location.
- Clearly identify the core without damaging it.

Filling Core Holes

- The hole made from the coring operation shall be filled with a material that will not become dislodged. If a bituminous material is available and used, it shall be compacted into the hole. A fast set concrete product may be used in lieu of a bituminous material.

Transporting Cores

- Transport cores on a smooth surface, top side down in a container(s) that prevents damage from jarring, rolling, hitting together, and/or impact with any object.
- Prevent cores from freezing or from excessive heat, 54° C (130° F), during transport.

Note #1: In extreme ambient temperature conditions, an insulated container should be used during transport.

- If the core is damaged to a point that it can not be utilized for its intended purpose the core will not be used for acceptance tests.

Separate the Layers

- When necessary to separate two or more pavement courses, lifts, or layers; separate by using a saw to cut the core on the designated lift line. Water must be sprayed on the saw blade to minimize the generation of excessive heat.

Note #2: Lift lines are often more visible by rolling the core on a flat surface.

Length Determination

- Measure the thickness of the designated lift to 3 mm. (0.1 in). Three or more measurements shall be taken around the core and averaged.

Report

- Core information shall be reported on standard agency forms. Include the following information:
 - The date the cores were obtained
 - Location of test and thickness of layer tested
 - The lift being evaluated
 - Type of material being evaluated
 - Mix Design Lab Number
 - Average thickness of each core (to the nearest 3 mm or 0.1 in.)

Addendum WAQTC TM 11

Following are guidelines for the use of WAQTC TM 11 by the State of Alaska DOT&PF.

1. While saw cutting is the preferred method, the different layers in a core may be separated by freezing and use of a chisel and hammer or by use of a hammer and chisel alone if a saw is not available. Care must be taken to protect the core from deformation or damage during the separation. If the core is deformed or damaged, it must be discarded and a new core taken.
2. Core locations – Joint cores shall be centered on the longitudinal joint. Mat cores shall be located at least 12” from all joints.
3. Core Locations – core locations shall be independent of other sampling.
4. When determining mat depth (thickness), determine and record the length (height) of the core to 5 mm (1/4”).
5. Damaged cores shall be replaced by cores located within 12” of the original test.
6. When material is sampled by other than DOT&PF personnel or their agent(s), the sampling must be witnessed and possession taken immediately by DOT&PF personnel or their agent(s).

Anti-Strip Requirements of Hot Mix Asphalt ATM 414

1. Scope

This method, an adaptation of AASHTO T 182, describes a procedure for determining the retention of a bituminous film by aggregate in the presence of water. It is applicable to asphalt cements, cutback asphalts and emulsified asphalts.

2. Apparatus

- Balance or scale: Capacity sufficient for the principle sample mass, readable to 0.1 percent of the total sample mass and meeting the requirements of AASHTO M 231.
- Thermostatically controlled oven capable of maintaining any required constant temperature between $49-150 \pm 1^\circ\text{C}$ ($120-300 \pm 1^\circ\text{F}$).
- A 9.5 mm ($\frac{3}{8}$ ") and a 4.75 mm (No. 4) mm sieve conforming to AASHTO M 92.
- 600 ml beakers, low form glass or plastic type.
- Thermostatically controlled water bath capable of maintaining a temperature of $49^\circ \pm 1^\circ\text{C}$ ($120^\circ \pm 2^\circ\text{F}$).
- Miscellaneous equipment including a steel spatula with stiff blade (approximately $\frac{1}{2}$ " wide x 4" long (25 mm x 100 mm), glass or plastic containers for mixing samples, and air-tight containers of suitable size for storing bitumen and anti-strip mixtures.

3. Sample Preparation

1. Aggregate:
 - a. The test aggregate shall be processed in the same manner as that which would be used during the construction process.
 - b. Dry the aggregate to a constant weight in accordance with WAQTC FOP for AASHTO T 255.
 - c. Separate the aggregate by sieving to obtain the minus 9.5 mm ($\frac{3}{8}$ ") plus (No.4) material. Reduce this material, in accordance with WAQTC FOP for AASHTO T 248, Method A, to obtain approximately 1200 g.
2. Anti-stripping additive used in testing will be the same brand and type proposed for use on the project.
3. Bitumen and/or emulsified asphalts will be the same type and grade proposed for use in mix design.

4. Procedure

1. For asphalt cement and/or cutback asphalt samples:
 - a. Thoroughly mix the bitumen samples with the anti-strip additive in the proportions of 0.25 percent, 0.50 percent, and 0.75 percent or as required. If necessary to store this mixture, use airtight containers.

Note 1: After the additive is added to the bitumen standards they shall not be reheated in excess of preheat temperatures as outlined in (1) and (2) below.
 - b. Make up 1 or more aggregate specimens per additive content by placing 100 ± 1 gram of the aggregate to be tested into individual mixing containers.
 - c. Preheat aggregate specimens to the temperature of the respective bitumen below:
 - (1) Asphalt cements: Preheat in oven at a temperature within the binders mixing temperature range for no longer than 30 minutes.
 - (2) Cut-back asphalts:
Grades 30 to 250. No preheat required.

Grades 800 to 3000: Preheat at 60-90°C (140-195 °F) for no longer than 30 minutes.

- d. Preheat the bitumen at the respective temperatures above until it can be poured.
- e. Add 5.5 ± 0.5 g of bitumen-additive mixture to the aggregate specimen(s).
- f. Mix the bitumen and aggregate thoroughly until uniformly coated.
- g. The bitumen-aggregate specimen(s) shall be oven-cured at a temperature $60 \pm 1^\circ\text{C}$ ($140 \pm 2^\circ\text{F}$) for a minimum of 18 hours but no more than 24 hours.
- h. Remove the sample(s) from the oven and re-mix to obtain a uniform coating. Allow the specimen(s) to cool to a temperature of 49°C (120°F) or less.
- i. Place 50 ± 1 g of each of the coated aggregates into individual 600 ml. beakers.
- j. Add 400 ml distilled water, cover and place in an oven or water bath maintained at $49^\circ \pm 1^\circ\text{C}$ ($120 \pm 2^\circ\text{F}$) for 24 hours. If a water bath is used, the container(s) shall not be submerged so as to allow bath water into the beakers.

2. For emulsified asphalts (anionic/cationic):

IMPORTANT: ANTI-STRIPPING ADDITIVE WILL NOT BE USED WITH EMULSIFIED ASPHALTS.

- a. Preheat the emulsified asphalt to $38 \pm 1^\circ\text{C}$ ($100 \pm 2^\circ\text{F}$). Mix the asphalt thoroughly.
- b. Make up 3 aggregate samples by placing 100 ± 1 g of the aggregate into individual containers.
- c. Preheat aggregate specimens to the emulsified asphalt preheat temperature listed in Step 1.c (2).
- d. Add 8.0 ± 0.5 g of each emulsion to the 100 g samples of aggregate and mix until the stones are uniformly coated.
- e. The emulsion-coated aggregate shall be cured at $132^\circ \pm 3^\circ\text{C}$ ($270 \pm 5^\circ\text{F}$) for a minimum of 18 hours but no more than 24 hours.
- f. Follow Steps 1.h thru 1.j.

5. Observations

1. Without disturbing or agitating the coated aggregate, remove any film floating on the water surface.
2. By observation through the water from above, estimate to the nearest 10 percent of the total visible surface area the aggregate coated with bitumen. Any thin brownish translucent areas are to be considered fully coated.
3. Average the results if more than one specimen was prepared for each additive content.

6. Report

Report the results on Department forms. The results will include the following:

- The visible bitumen/emulsion-covered area estimated to the nearest 10 percent for each additive content tested.
- The lowest percentage of additive required to obtain a 70 percent bitumen coating on the aggregate.
- Type and grade of bitumen/emulsion used.
- Brand of anti-stripping agent use.

Hot Mix Asphalt Design by the Marshall Method ATM 417

1. Scope

This method describes the Marshall Mix Design procedure for determining the optimum asphalt content, stability, flow and void properties of hot bituminous mixtures containing; aggregates with maximum sizes of (1") or less, Recycled Asphalt Pavements (RAP) , mixes utilizing rubber, and Warm Mix Asphalt (WMA). As recommended by AASHTO R 12, this method is adapted from the Asphalt Institute "Mix Design Methods for Asphalt Concrete and Other Hot Mix Types", Manual Series No. 2 (MS-2). It also includes information and procedures from AASHTO T 245 and AASHTO R 30Apparatus

- Ovens and hot plates thermostatically controlled to maintain the various required temperatures within $\pm 3^{\circ}\text{C}$ (5°F).
- Temperature measuring devices:
For asphalt cement and mixes: having a range of $10\text{--}200^{\circ}\text{C}$ ($50\text{--}400^{\circ}\text{F}$) and sensitive to 3°C (5°F).
For the water bath: readable and sensitive to $\pm 0.2^{\circ}\text{C}$ (0.5°F) at 60°C (140°F).
- Balance or scale: Capacity sufficient for the principal sample mass, readable to 0.1 percent or 0.1 g of the total sample mass and meeting the requirements of AASHTO M 231.
- Sieve shaker meeting the requirements of WAQTC FOP for AASHTO T 27/T 11.
- Mechanical mixer with a wire whip mixing blade capable of producing a well coated, homogeneous mixture and mixing bowls. Means of maintaining the mixture at mixing temperature, such as a heat lamp mounted below the mixer.

Note 1: The Hobart Kitchen Aid Model K-5A with wire whip Model K5A-WW has been found satisfactory.

- The mold assemblies, compaction pedestal, mold holder, extruder, breaking head and flow meter or stress-strain recorder shall conform to AASHTO T 245.
- If rubber is being used in the mix, weights of at least 5 lbs in mass and slightly smaller than 4-inches in diameter will be required. The weights should be of such diameter to loosely fit inside the 4-inch Marshall molds.
- Mechanical compaction device conforming to AASHTO T 245. The device shall be equipped with a counter that will automatically shut off the machine at the required number of blows. The device will be calibrated annually in accordance with ASTM D 2168.
- Paper discs of heavy weight non-absorbent paper stock, 100 mm (4") diameter.

Note 2: The Humboldt H-1341P paper disc has been found satisfactory.

If rubber is being used in the mix, substitute acetate discs for the paper discs. Hewlett Packard overhead transparency film (HP 92296T) has been found to work well.

- The water bath shall be at least 150 mm (6") deep and shall be thermostatically controlled so as to maintain a temperature of $60 \pm 1^{\circ}\text{C}$ ($140 \pm 1.8^{\circ}\text{F}$). The bath shall be equipped with an agitator to keep the water in constant circulation. It shall have a perforated false bottom or shelf for supporting the specimens a minimum of 2" (50 mm) above the bottom of the bath. The bath shall have a flat surface area large enough to allow the specimens to set singly with water flowing freely around each specimen. Stacking specimens is prohibited.
- Loading jack consisting of either a motor-driven screw jack, a hydraulic jack or other mechanical loading

device which shall produce a uniform loading head movement rate of 50 mm (2") per minute, independent of the load being applied. The loading frame shall have a minimum load capacity of 25 KN (5000 lb).

- Load measuring device of 25 KN (5000 lb) minimum capacity, sensitive to 50 N (10 lb) or less, and capable of measuring displacement to 0.0025 mm (0.0001"). This device may be a load-cell or a ring dynamometer assembly.
- Flowmeter—the flowmeter shall consist of a guide sleeve and a gage. The activation pin of the gage shall slide inside the guide sleeve with a slight amount of frictional resistance. The guide sleeve shall slide freely over the guide rod of the breaking head. The flowmeter gage shall be adjusted to zero when placed in position on the breaking head when each individual test specimen is inserted between the breaking head segments. Graduations of the flowmeter gage shall be in 0.25 mm (0.01") divisions.
- Data measuring/recording/display devices capable of the capacity and sensitivity of the load-measuring device and or flowmeter.
- Miscellaneous equipment including scale or caliper readable to 0.25 mm (0.01"), sample containers (metal pans, bowls or beakers), spatulas, spoons, marking crayons, heat resistant gloves, straight-edge, etc.
- Bituminous Mix Design Worksheet, Bituminous Mix Design Report, and 0.45 Gradation Chart paper.

2. Synopsis

Aggregate properties important to bituminous mixes shall be determined as required. For Hot Mix Asphalt (HMA) mixes this will include: gradation of each submitted aggregate and, after combining according to the proposed Job Mix Formula (JMF), the plasticity index, fracture, flat & elongated, and bulk specific gravity of the coarse & fine aggregate. For Stone Mastic Asphalt (SMA) mixes, in addition to the tests listed for HMA mixes, the unit mass of the combined coarse aggregate and the apparent specific gravity of the mineral filler will be required.

A minimum of four (4) sets of three (3) specimens each, shall be prepared, mixed and compacted at different asphalt contents. These asphalt contents shall be by mass of total mix and will be at 0.5 percent increments. These specimens will be tested for Unit Mass, Marshall Stability & Flow, Percent Air Voids in Total Mix (VTM), Percent Voids in Mineral Aggregate (VMA), Percent Voids Filled with Asphalt (VF), and (for SMA mixes) Voids in Coarse Aggregate (VCA). The final results will define the VTM over that parameters specification range and should define the maximum values of the Stability and Unit Mass of the mix and the minimum value for VMA.

Three (3) specimens shall be prepared, mixed and tested to determine the maximum specific gravity in accordance with WAQTC FOP for AASHTO T 209.

Calibration specimens will be prepared as required by the Acceptance testing program for the project. The calibrations may include any of the following:

- JMF Calibration Points for the Nuclear Asphalt Content Gauge for ATM 405.
- Ignition Furnace Calibration Points for each Ignition Furnace System for WAQTC FOP for AASHTO T 308.

When RAP is incorporated in the mix design, an extraction device as described in AASHTO T 164 is required to determine the asphalt content and the aggregate properties of the RAP proposed for use in the mix. The contractor will submit asphalt content and gradations from 10 representative samples collected from the proposed RAP source. The contractor will submit 3 representative samples to be tested for verification of the contractors asphalt content and gradation properties for the stockpile.

The Theoretical Maximum Specific Gravity will be determined on a representative portion of the RAP, in

accordance with AASHTO T 209. The effective specific gravity will be used as RAP aggregate bulk specific gravity, for mix designs that incorporate more than 15% RAP in the mix. With mixes containing 15% or less RAP use the virgin aggregate specific gravities.

3. Determination of Asphalt Cement Properties

If not provided by the supplier, determine the following:

- 4.1 Verify compliance of the asphalt cement plus additives to specifications; in addition, determine the specific gravity at 25°C (77°F) of the asphalt cement in accordance with AASHTO T 228/ASTM D 70.
- 4.2. Establish the temperature-viscosity properties of the cement in accordance with ASTM D 2493 with the viscosities determined in accordance with the following as required by the project specifications:

AASHTO T 201 & T 202 Or AASHTO T 315 & T 316
ASTM D 2170 & D 2171

- 4.3 Select the mixing and compaction temperatures using the temperature-viscosity data. Determine, unless otherwise specified, the mixing temperature at 170 ± 20 centistokes and the compaction temperature at 280 ± 30 centistokes.

Note 3: Modified asphalts may not adhere to the equiviscosity requirements noted; the manufacturer's recommendations should be requested and used to determine mixing and compaction temperatures. Practically the mixing temperature should not exceed 165°C (330°F) and the compaction temperature should not be lower than 115°C (240°F).

4. Determination of Rubber Properties

- 5.1 Perform a gradation of the rubber product in accordance with WAQTC FOP for AASHTO T 27/T 11. Washing is not required.
- 5.2 Obtain the specific gravity of the rubber from the manufacturer.

5. Preparation of Aggregate

The aggregates used for the mix design will represent the aggregates in the contractor's stockpiles. The laboratory will use the aggregate as presented by the contractor and prepare the aggregate in the same manner as it will be handled during production. In no event will the aggregate be washed in the preparation of any test specimens other than the dust correction procedure.

RAP shall be considered an aggregate for the purposes of batching material. The oil content of RAP will be considered asphalt cement. Virgin aggregate and cement will be adjusted accordingly. Dry RAP at temperatures less than 60° C prior to use. RAP will be added to the aggregate at time of batching.

- 6.1 Mix the aggregates from the individual stockpiles at the blend ratio specified by the contractor.

Separate the combined aggregates by dry sieving into individual specification sieve sizes including the minus 75 µm (No. 200) material. As the material is being dry sieved, separation will not be as efficient as when using washed samples. Therefore sieving time must be increased to separate as efficiently as possible. Sieving times should be increased to 15 minutes for coarse aggregate separation and 15-20 minutes for fine aggregate. The increased sieving time may be determined in accordance with WAQTC FOP for AASHTO T 27/T 11 (See Note 5).

Separate sufficient aggregate to perform all required tests (i.e. Marshall Stability, Calibration Points for Nuclear Content Gauge, Ignition Furnace, and aggregate properties as required).

- 6.2 Using the contractor proposed gradation calculate the initial cumulative masses for each specification sieve

size by the following:

$$X = \frac{(100 - P_N)}{100} \times E_i$$

where:

X = Cumulative aggregate batch masses for sieve size N, record to the nearest 1 g,

P_N = Percent passing from proposed gradation for sieve size N, and

E_i = Initial total aggregate mass for a Marshall specimen.

Note 4: The initial aggregate mass may be chosen based on experience or a mass such as 1200 g may be assumed at this point. If a mass is assumed, a trial specimen to determine if height adjustment in accordance with the methodology of Preparation of Test Specimens, Step 1 a thru c will be required.

6.3 Aggregate Batching Correction:

As the JMF gradation was determined in accordance with WAQTC FOP for AASHTO T 27/T 11, which washed the sample in some manner, and the material for the mix design has been separated by dry sieving which will not completely separate the aggregate, a correction must be made to the material separated for the mix design to ensure that the proper amount of aggregate but especially the minus 75 µm (No. 200) material is included in the test specimens. If this is not done, batching material in accordance with the methodology outlined in this method will result in the mix design having a higher percentage of aggregate, fine sand and/or silt than the contractor's JMF proposes.

- a. Prepare a wash gradation sample.

Calculate the initial batch masses for the wash gradation.

- b. Perform a wash gradation in accordance with WAQTC FOP for AASHTO T 27/T 11.
- c. Compute the adjusted cumulative batch masses for each of the sieve sizes by the following formula:

$$Z_{Ni} = \frac{X^2}{Y}$$

where:

Z_{Ni} = corrected cumulative batch mass for sieve size N,

X = pre-wash cumulative batch mass for sieve size N,

Y = post-wash cumulative batch mass for sieve size N.

Note 5: In some cases, the adjusted cumulative batch masses will result in decreasing batch masses instead of increasing batch masses. This indicates that the dry sieving operation did not efficiently separate the fine aggregate, leaving too much 75 µm (No. 200) and minus 75 µm (No. 200) material in the larger aggregate sizes. If this occurs, resieve the sizes showing the decreasing batch masses, combining the separated material with the material already separated and perform Step 6.3 a thru c again.

- d. Tabulate the overall adjusted cumulative batch.

6.4 Prepare samples from the separated aggregate for the determination of the:

- Plastic Index in accordance with WAQTC FOP for AASHTO T 90,
- Percentage of Fracture in Coarse Aggregate in accordance with WAQTC FOP for AASHTO T 335,
- Unit weight of fine and coarse aggregate in accordance with T 84 and WAQTC FOP for AASHTO T 85 respectively,
- Flat and elongated Particles in accordance with ATM 306, if required, and
- Sand Equivalent in accordance with WAQTC FOP for AASHTO T 176, if required.

6. Estimate Projected Optimum Asphalt and Rubber Content

7.1 Estimate the projected optimum asphalt content. This value can be based on any or all of these sources:

- a. Experience. This is the most important method of estimating projected optimum asphalt content. The projected optimum asphalt content will be estimated to the nearest 0.5 percent with four (4) sets of three (3) specimens prepared to bracket the projected optimum at 0.5 percent intervals.

The following methods may be used where no experience exists for the proposed material and/or JMF target values.

- b. Computational formula:

$$P = 0.035a + 0.045b + Kc + F$$

where:

P = projected optimum asphalt content of mix, percent by mass of mix,

a = percent retained on the 2.36 mm (No. 8) sieve, expressed as a whole number

b = percent passing the 2.36 mm (No. 8) sieve minus the percent passing on the 75 µm (No. 200) sieve, expressed as a whole number

c = percent passing the 75 µm (No. 200) sieve, expressed to the 0.1 percent

K = 0.15 for 11 to 15 percent passing the 75 µm (No. 200) sieve, or

0.18 for 6 to 10 percent passing the 75 µm (No. 200) sieve, or

0.20 for 5 percent or less passing the 75 µm (No. 200) sieve, and

F = asphalt absorption. In the absence of other data, use 0.7 percent.

The projected optimum asphalt content will be rounded to the nearest 0.5 percent with specimens prepared as indicated under step 1.a.

- c. Dust-Asphalt Ratio: Since the Dust-Asphalt Ratio specification is typically 0.6 to 1.2, using the larger of the D/A limits will give the projected minimum *effective* asphalt content for the JMF p200 target. Solving the Dust-Asphalt ratio formula for the projected minimum asphalt content percent (effective asphalt content plus absorbed asphalt):

$$\text{Max. D/A} = \left(\frac{p200}{P} \right)$$

$$\text{for P results in } P = \left(\frac{p200}{\text{Max.D / A}} \right)$$

where:

P = projected minimum *effective* asphalt content of mix, percent by mass of mix,

p200 = percent passing the 75 µm (No. 200) sieve, and

Max. D/A = dust-to-asphalt ratio.

The total projected asphalt content may be estimated by:

$$P_m = P + F$$

where:

P_m = projected minimum asphalt content, percent

P = projected minimum effective asphalt content of mix, percent

F = asphalt absorption, percent. In the absence of other data use 0.7 percent.

- d. Percent rubber will be determined by the Regional Materials Engineer. Rubber will be calculated as a percent of aggregate.

This projected minimum asphalt content will be rounded to the nearest 0.5 percent with specimens prepared for at this projected minimum value and at least three (3) more above this value at 0.5 percent intervals.

7. Preparation of Test Specimens

8.1 Marshall Stability and Flow: Batch a minimum of four (4) sets of three (3) aggregate specimens each.

However, if the initial total aggregate mass for the Marshall specimen was estimated without prior experience, a single Marshall specimen will be batched, mixed at the projected optimum asphalt content, compacted and the thickness of the compacted specimen measured to determine if the aggregate mass must be adjusted. If rubber is used in the mix it will be added at this time.

a. Thickness Adjustment

- 1) The height of the compacted specimen must be within the specimen thickness limitations of 62-65 mm (2.45-2.55"). If it is not, adjust the total mass of the aggregate as shown below and recalculate the individual sieve masses to bring the specimens within this range.
- 2) Prepare an aggregate batch to the masses calculated above and calculate the mass of asphalt required for the estimated optimum asphalt content as shown below. Mix and compact the trial specimen in accordance with the requirements of sections **9** and **11**.
- 3) If thickness adjustment is necessary, adjust E_i , the initial total aggregate mass, by the following:

$$E_a = \frac{2.5 \times E_i}{H} \text{ (USC) or } \frac{63.5 \times E_i}{H} \text{ (SI)}$$

where:

E_a = adjusted total aggregate mass,

E_i = initial total aggregate mass, and

H = specimen thickness 0.1 mm (0.01") actually obtained.

- 4) If necessary, adjust each Z_{Ni} from Step 6.3c by:

$$Z_{Na} = \frac{E_a}{E_i} \times Z_{Ni}$$

where:

Z_{Na} = adjusted cumulative batch mass for sieve size N,

E_a = adjusted total aggregate mass,

E_i = initial total aggregate mass,

Z_{Ni} = corrected cumulative batch mass for sieve size N.

- 5) Using either the corrected cumulative sieve masses (Z_{Ni}) determined in **Preparation of Aggregate**, Step 6.4c or the adjusted cumulative sieve masses (Z_{Na}) determined in Step 1a, above, prepare three (3) aggregate specimens for each asphalt content. The aggregate for each specimen will be batched and placed in a container and dry-mixed thoroughly.

- b. Calculate the mass of the asphalt cement for each set of specimens by:

$$AW = \frac{E_i \text{ (or } E_a) \times P_{bN}}{100 - P_{bN}}$$

where:

AW = mass of asphalt cement, to the nearest 0.1 g,

E_i (or E_a) = initial (or adjusted, see below) aggregate mass, and

P_{bN} = asphalt content for set N, to the nearest 0.1 percent.

8.2 Maximum Specific Gravity of Mixture.

- a. For each sieve size, calculate the cumulative masses for a maximum specific gravity (Rice) test specimen by the following formula:

$$R_N = \frac{Q}{E_i} \times Z_{Ni}$$

where:

R_N = cumulative batch mass for the maximum specific gravity specimen for sieve size N,

E_i = initial total aggregate mass,

Z_{Ni} = corrected cumulative batch mass for sieve size N, and

Q = minimum sample mass required by WAQTC FOP for AASHTO T 209.

- b. Prepare three (3) test specimens to these masses for performance of WAQTC FOP for AASHTO T 209.

8.3 Coarse Aggregate Properties.

- a. For each coarse aggregate sieve size, calculate the cumulative masses for the required test specimens of coarse aggregate for the required test procedures by the following formula:

$$C_N = \frac{Q}{\text{No. 4 } Z_N} \times Z_{Ni}$$

where: C_N = cumulative batch mass for the maximum specific gravity specimen for sieve size N, for the 4.75 mm (No. 4) and larger sieves only,

Q = minimum sample mass required for the required tests.

$\text{No. 4 } Z_N$ = initial total aggregate mass of 4.75 mm (No. 4), and

Z_{Ni} = adjusted cumulative batch mass for sieve size N.

- b. Prepare the required number of test specimens to the minimum sample size required by the test procedure for the performance of the following or other specified tests as required:

<u>Test Procedure</u>		<u>Number of Specimens</u>
<u>Designation</u>	<u>Title</u>	
WAQTC FOP for AASHTO T 85	Specific Gravity	1
WAQTC FOP for AASHTO T 335	Fracture	1
ATM 306	Flat-Elongated	1
AASHTO T 19 (SMA only)	Bulk Density	3

8.4 Fine Aggregate Properties.

- a. For each fine aggregate sieve size, calculate the cumulative masses for the specific fine aggregate property test by the following formula:

$$F_N = \left(\frac{Q}{E_i - Z_{4i}} \right) \times (Z_{Ni} - Z_{4i})$$

where:

F_N = cumulative batch mass for the fine aggregate specific gravity specimen for sieve size N, for the minus 4.75 mm (No. 4) sieves only,

Q = sample mass required for the specified test,

- E_i = initial total aggregate mass,
 Z_{Ni} = initial cumulative batch mass for sieve size N, and
 Z_{4i} = initial cumulative batch mass for the 4.75 mm (No. 4) sieve.

- b. Prepare the required number of test specimens to the minimum sample size required by the test procedure for the performance of the following or other specified tests as required:

<u>Test Procedure</u>		<u>Number of Specimens</u>
<u>Designation</u>	<u>Title</u>	
WAQTC FOP for AASHTO T 90	Plastic Index	1
AASHTO T 84	Specific Gravity	3
WAQTC FOP for AASHTO T 176	Sand Equivalent	1

8.5 Mineral Filler Specific Gravity.

If the JMF p200 is greater than 6 percent, the minus 75 μ m (No. 200) material will be treated as mineral filler and the apparent specific gravity of this material will be determined in accordance with AASHTO T 100.

8. Preparation of Asphalt Cement

Heat a minimum of 1 L (1 qt) of asphalt cement to the mid-point of the mixing temperature range.

It is best to use the asphalt cement as soon as it reaches mixing temperature. If this is not possible, maintain the asphalt cement at this temperature in a covered container rather than reheat it.

9. Preparation of Mixtures and Mixture Conditioning

- 10.1 Place the aggregate specimens for Marshall Stability & Flow and Maximum Specific Gravity in the oven and heat to the mid-point of the asphalt cement mixing temperature range.
- 10.2 "Butter" the mixing bowl with asphalt cement and fine aggregate mixture that will coat the mixing area of the bowl. Remove any excess material.
- 10.3 Place the heated specimen into the mixing bowl.
- 10.4 Form a crater in the dry blended aggregate large enough to hold the asphalt cement, place the mixing bowl on the scale and weigh into the aggregate crater, to the nearest 0.1 g, the required amount of pre-heated asphalt cement.
- 10.5 Mechanically mix the aggregate and asphalt cement rapidly until thoroughly coating the aggregate and return to the oven.
- 10.6 After mixing, spread the mixture in a pan to an even thickness of 25-50 mm (1-2 inches). Place the mixture and pan in a forced-draft oven at the midpoint of the compaction temperature range for 120 ± 5 minutes. Stir the mixture after 60 ± 5 minutes to maintain uniform conditioning. Highly absorptive aggregates may require a longer conditioning time.

10. Equipment Preparation

- 11.1 Thoroughly clean the mold assemblies (molds, bases and collars) and heat in an oven to the mid-point of the asphalt cements compaction temperature range.
- 11.2 Thoroughly clean the face of the compaction hammer and heat on a hot plate to a temperature within the asphalt cements compaction temperature range.

11. Compaction of Specimens

- 12.1 Place the pre-heated mold assembly into the mold holder on the compaction pedestal. Place a paper disc, or acetate disc if rubber is used in mix, in the bottom of the mold.
- 12.2 Stir the specimen thoroughly and place in the mold. Spade the mixture vigorously with a heated spatula 15 times around the perimeter and 10 times over the interior, remove the collar and smooth the surface of the mix to a slightly rounded shape.
- 12.3 Place a paper disc, or acetate disc if rubber is used in mix, on top of the specimen, position the compaction hammer, and apply the required number of blows with the compaction hammer.
- 12.4 Remove the base plate and collar, invert and re-assemble the mold, and apply the same number of blows to the face of the inverted specimen.
- 12.5 Remove the collar, base plate and paper discs, mark each biscuit for individual identification, and allow them to cool until the specimen can be extruded without damage or distortion.

If rubber is used in the mix, do not remove the base plate or acetate discs. Place a minimum 5lb mass on top of specimen and let stand 24 hours. After 24 hours remove weight.
- 12.6 Extrude the specimen from the mold; transfer to a smooth, flat surface; allow it to stand and cool to room temperature. Acetate discs can be removed at this point. Specimens can be placed on a hot plate for a few seconds to facilitate removal.

12. Mix Sample Test Procedures

- 13.1 Measure and record the thickness of each compacted specimen and record to the nearest 0.25 mm (0.01"). Use either a device that will measure the average height or measure the height with a caliper at three (3) locations spaced evenly around the circumference of the specimen and average these results.
- 13.2 Determine the bulk specific gravity of each compacted specimen in accordance with WAQTC FOP for AASHTO T 166/T 275.
- 13.3 Stability and Flow.
 - a. Bring the specimens to the specified temperature of $60 \pm 1^{\circ}\text{C}$ ($140 \pm 1.8^{\circ}\text{F}$) by immersing in the water bath for 30 to 40 minutes. Stacking specimens on top of each other is prohibited.
 - b. Thoroughly clean and lubricate the guide rods, and clean the inside surfaces of the breaking heads before performing the stability and flow tests. Maintain the breaking head at a temperature of 21 to 38°C (70 to 100°F).
 - c. Remove the specimens one at a time from the water bath and place in the lower segment of the breaking head.
 - d. Place the upper segment of the breaking head on the specimen, firmly seat the head on the specimen, and place the complete assembly in position on the loading jack.

The elapsed time for the test from the removal of the test specimen from the water bath to the maximum load determination shall not exceed 30 seconds.
 - e. For machines using proving ring & flow meter:
 - 1) Place the flow meter over one of the guide rods and adjust the flow meter to zero; hold the sleeve firmly against the upper segment of the breaking head while the test load is applied.
 - 2) When the load to the specimen at a constant rate of 50.8 mm (2") per minute until the maximum load is reached. The maximum load is indicated when the proving ring dial value decreases.
 - 3) Simultaneously read the proving ring dial to the nearest 0.0025 mm (0.0001") and the flow meter to

the nearest 0.25 mm (0.01"). Record the readings as whole numbers (no decimal points) from the proving ring dial flow meter.

- f. For machines using load cell and chart recorder/display:
 - 1) Turn on the recorder, adjust the pen to the zero position according to the manufacture's instructions, turn the range selector to the appropriate range (use the smallest range possible) and set the chart speed at 10" per minute (250 mm per minute).
 - 2) Apply the load to the specimen by means of the constant rate movement of the loading jack at 50 mm per minute (2" per minute) until the maximum is reached and the load, as indicated by the chart recorder, decreases.

4. Maximum Specific Gravity.

Determine the maximum specific gravity of the prepared specimens at or near the optimum asphalt content in accordance with WAQTC FOP for AASHTO T 209 as follows:

- a. Choose a projected optimum asphalt content as described in **Estimate Projected Optimum Asphalt Content**.
- b. Mix and condition the specimens in accordance with the provisions of **Preparation of Mixtures and Mixture Conditioning**.
- c. Determine the maximum specific gravity in accordance with WAQTC FOP for AASHTO T 209 on the prepared specimens at the projected optimum asphalt content.
- d. If the projected optimum asphalt content differs from the final optimum asphalt content, determined below in **Determination of Optimum Asphalt Content, Selection of Final Optimum Asphalt Content**, by 1 percent or more, prepare and determine a new maximum specific gravity at the final optimum asphalt content and recalculate the maximum specific gravities at the other asphalt contents, the voids total mix and the optimum asphalt content.

13. Calculations

- 14.1 Calculate the bulk specific gravity of each compacted specimen in accordance with WAQTC FOP for AASHTO T 166/T 275. Average the bulk specific gravities (G_{mb}) of all compacted specimens for each asphalt cement content.

Record the result to the nearest 0.001.

- 14.2 Calculate the unit weight for each asphalt content by:

$$W_N = G_{mbN} \times 997.1 \text{ kg/m}^3 \text{ (62.245 lb/ft}^3\text{)}$$

where:

W_N = unit weight of set N,

G_{mbN} = average bulk specific gravity of set N, and
997.1 kg/m³ (62.245 lb/ft³)=density of water at 25°C (77°F).

Record the result to the nearest 1 kg/m³ (0.1 lb/ft³).

- 14.3 Calculate the maximum specific gravity of the mix at the selected asphalt content in accordance with WAQTC FOP for AASHTO T 209. Average the results and record the average to the nearest 0.001.
- 14.4 Calculate the maximum specific gravity for each asphalt content as follows:
- a. Calculate the effective specific gravity of the aggregate by:

$$G_{se} = \frac{100 - P_b}{\frac{100}{G_{mm}} - \frac{P_b}{G_b}}$$

where:

G_{se} = effective specific gravity of the aggregate,

P_b = asphalt content at which G_{mm} was determined,

G_{mm} = maximum specific gravity at P_b ,

G_b = specific gravity of the asphalt at 25 °C (77°F).

Record the result to the nearest 0.001.

- b. Calculate the maximum specific gravity for each asphalt content by:

$$G_{mm} = \frac{100}{\frac{100 - P_{bN}}{G_{se}} + \frac{P_{bN}}{G_b}}$$

where:

G_{mm} = maximum specific gravity for asphalt content P_{bN} ,

G_{se} = effective specific gravity of the aggregate,

P_{bN} = percent asphalt for set N, and

G_b = specific gravity of the asphalt at 25 °C (77°F).

Record the result to the nearest 0.001.

- 14.5 Calculate the percent air voids in total mix (VTM) for each asphalt content by:

$$VTM = \frac{G_{mm} - G_{mb}}{G_{mm}} \times 100$$

where:

VTM = percent voids total mix,

G_{mb} = average specific gravity of each content, and

G_{mm} = maximum specific gravity of each content.

Record the result to the nearest 0.1 percent.

- 14.6 Calculate the percent voids in mineral aggregate (VMA) for each asphalt content by:

- a. Calculate the blended aggregate bulk specific gravity by:

$$G_{sb} = \frac{100}{\frac{P_1}{G_1} + \frac{P_2}{G_2} + \dots + \frac{P_N}{G_N}}$$

where:

G_{sb} = blended aggregate bulk specific gravity,

$P_1, P_2 \dots & P_N$ = percent of individual aggregate,

$G_1, G_2 \dots & G_N$ = bulk specific gravity individual aggregate.

Record the result to the nearest 0.001.

- b. Calculate the percent voids in mineral aggregate for each asphalt content by:

$$VMA = 100 - \frac{G_{mb} (100 - P_b)}{G_{sb}}$$

where:

- VMA = percent voids in mineral aggregate for each content,
- G_{sb} = blended aggregate bulk specific gravity,
- G_{mb} = average bulk specific gravity for each content, and
- P_b = percent asphalt of each content.

Record the result to the nearest 0.1 percent.

- 14.7 Calculate the percent voids filled with asphalt (VFA) for each asphalt content by:

$$VFA = 100 \times \frac{VMA - VTM}{VMA}$$

where:

- VFA = percent voids filled with asphalt for each content,
- VMA = percent Voids in mineral aggregate for each content, and
- VTM = percent voids total mix for each content.

Record the result to the nearest whole percent.

- 14.8 Calculate the dust/asphalt ration for each asphalt content by:

- a. Calculate the asphalt absorption by:

$$P_{ba} = 100 \left(\frac{G_{se} - G_{sb}}{G_{sb} \times G_{se}} \right) G_b$$

where:

- P_{ba} = absorbed asphalt, percent by mass of aggregate,
- G_{se} = effective specific gravity of aggregate,
- G_{sb} = bulk specific gravity of aggregate, and
- G_b = specific gravity of asphalt.

- b. Calculate the effective asphalt content for each asphalt content by:

$$P_{be} = P_b - \left(\left(\frac{P_{ba}}{100} \right) \times (100 - P_b) \right)$$

where:

- P_{be} = effective asphalt content, percent by total mass of mix,
- P_b = asphalt content, percent by total mass of mix, and
- P_{ba} = absorbed asphalt, percent by mass of aggregate.

- c. Calculate the dust/asphalt ratio by:

$$D/A = \frac{p_{200}}{P_{be}}$$

where:

- D/A = dust/asphalt ratio,
- p_{200} = percent passing the 75 μ m (No. 200) sieve, and
- P_{be} = effective asphalt content, percent by total mass of mix.

14.9 Stability:

- a. For machines using proving ring and flow meter, calculate the uncorrected stability from the dial readings by the following:

$$S = (D \times m) + C$$

where:

- S = uncorrected stability load, in pounds,
D = dial reading as a whole number
m = slope from proving ring calibration, and
C = constant from proving ring calibration.

Record the result to the nearest whole pound.

- b. For machines using load cell and chart recorder/display, read and record the uncorrected stability to the accuracy allowed by the chart scale.
- c. Stability values for each specimen that differ from the standard 63.5 mm (2.5") thickness will be corrected to the equivalent 63.5 mm (2.5") value by the following:

$$CS = S \times t$$

where:

- CS = corrected stability,
S = uncorrected stability, and
t = thickness correction factor = $-0.64x + 2.6$ for x in inches or $-0.025x + 2.5875$ for x in mm.
(Equations derived from data presented in Table 2 of AASHTO T 245 for thicknesses from 2.4375" to 2.5625" (61.9 mm to 65.1 mm).)

TABLE 1
Thickness Correction Factors

Inches	mm	t-Correction Factor
2.45	62.2	1.03
2.46	62.5	1.03
2.47	62.7	1.02
2.48	63.0	1.01
2.49	63.2	1.01
2.50	63.5	1.00
2.51	63.8	0.99
2.52	64.0	0.99
2.53	64.3	0.98
2.54	64.5	0.97
2.55	64.8	0.97

Table based on data from AASHTO T 245 Table 2

- d. Corrected stability values for each asphalt content averaged and recorded to the nearest 50 N (10 lb).

Flow:

- a. For machines using the proving ring and flow meter, average the flow values for each asphalt content and record as a whole number (e.g. flow reading of 0.12 will be recorded as 12).

- b. For machines using load cell and chart recorder:
 - 1) Extend the constant rate slope line to intersect the horizontal axis.
 - 2) Determine the maximum load point and draw a line perpendicular to the horizontal axis through this point to intersect the horizontal axis.
 - 3) From the point determined in (1) to the point determined in (2), read and record the flow as a whole number in 0.01" increments.
 - 4) Average the flow values for each asphalt content set and record to the nearest whole number.

14. Determination of Optimum Asphalt Content

For a mix to satisfy a specific project specifications graphical presentation of the results should be prepared prior to the selection of the optimum asphalt content.

Graphical Presentation:

Prepare a graphical plot of Asphalt Content vs. Unit Weight, Stability, Flow, Percent Voids Total Mix, Percent Voids in Mineral Aggregate, and Percent Voids Filled with a smooth curve that represents a best-fit for all values.

15.1 Determination of Optimum Asphalt Content:

- a. Determination of Preliminary Optimum Asphalt Content: Choose the preliminary optimum asphalt content at the median of the Voids in Total Mix specification. All of the calculated and measured mix properties should then be evaluated by comparing them to the project mix design specifications. If all of the specifications are met, then this is the preliminary optimum asphalt content. If all of the specifications are not met, then some adjustment or compromise is necessary or the mix may need to be redesigned. Even if all of the specifications are met, a number of considerations should be evaluated before choosing the final optimum asphalt content.
- b. Selection of Final Mix Optimum Asphalt Content: The final optimum asphalt content should be a compromise selected to balance all of the mix properties. Normally, the mix design specifications will produce a narrow range of acceptable asphalt contents that will pass all specifications. The asphalt content selection can be adjusted within this narrow range to achieve establishing the final optimum asphalt content. Establishing a final optimum asphalt content is covered in detail in Asphalt Institute Manual MS-2, 6th Edition, Mix Design Methods, Chapter 5, Marshall Mix Design Method, Section D-5.15, Selection of Final Mix Design, pages 69 thru 77.

If this evaluation reveals no asphalt content which meets all project specifications or such a narrow range of asphalt contents meeting all project specifications as to be unfeasible and/or uneconomical to produce, the Materials Engineer may reject the proposed job mix design and require a new proposed job mix formula from the contractor.

15. Report

The report shall include the following:

- Project identification, Source/Supplier of mix and name of the general contractor.
- Aggregate quality identification(s), target gradation, blend ratio of individual stockpiles, blended bulk specific and effective specific gravities. Other properties that may be specified in the Contract such as: fineness modulus of the blended fine aggregate; percent fracture; percent flat and elongated; and the plasticity index of the blended fine aggregate.
- Asphalt cement quality identification, specific gravity at 77°F, and the maximum mixing temperature.

- Anti-strip additive brand/type and the minimum percent required.
- Asphalt content at the median of the percent voids in total mix specification and the approved optimum asphalt content.
- The following properties at the optimum asphalt content: maximum specific gravity, percent voids in total mix, percent voids in mineral aggregate, percent voids filled, stability, flow, unit mass and the dust-asphalt ratio.
- Graphical representation on a 0.45 power graph of the target gradation with the Lower Specification Limit (LSL)-Upper Specification Limit (USL).
- Graphical representation of asphalt content versus the following properties: unit weight, stability, flow, percent voids in total mix, percent voids in mineral aggregate and voids filled.
- Identification and address of the laboratory that performed the mix design, that laboratory's mix design identification number and the signature/title of the professional engineer who reviewed and approved/disapproved the mix design.

Appendix ATM 417

1. Example Calculations

(See Example Worksheets.)

See Section 8 of the standard for definitions of the variables.

Contractor Proposed JMF for a Type IIA HMA Mix Design

Sieve	Percent Pass.	
3/4"	100	
1/2"	89	Note: Nominal Maximum Size
3/8"	76	of this material is 3/4 inch.
#4	52	
#8	36	
#16	24	
#30	15	
#50	9	
#100	7	
#200	5.1	

TABLE 2

Sieve Size	Job Mix Formula	PreWash Mass
3/4"	100	0
1/2"	89	129
3/8"	76	282
#4	52	564
#8	36	752
#16	24	893
#30	15	999
#50	9	1069
#100	7	1093
#200	5.1	1115
-#200	0	1175

2. Preparation of Aggregate

2.1 Initial total aggregate mass: $E_i = 1175.0$ g

Calculate cumulative aggregate batch mass by:

$$x = \frac{100 - \text{Percent Passing}}{100} \times E_i$$

$$\text{for No. 4} = \frac{100 - 52}{100} \times 1175.0 = 564 \text{ g}$$

$$\text{for No. 8} = \frac{100 - 36}{100} \times 1175.0 = 752 \text{ g}$$

$$\text{for No. 200} = \frac{100 - 5.1}{100} \times 1175.0 = 1115 \text{ g}$$

Repeat for the other required sieve sizes.

2.2. Aggregate Batching Correction

- Prepare a sample by batching a specimen with cumulative masses corresponding to cumulative aggregate batch masses calculated above, see the Pre Wash Mass column of Table 2.
- Wash and sieve this prepared sample in accordance with WAQTC FOP for AASHTO T 27/T 11. Record the cumulative mass on the sieves in a Post Wash Column, see Table 3.
- Calculate the adjusted cumulative batch mass for each sieve as follows, See Table 4 for other sieves:

TABLE 3

Sieve Size	Job Mix Formula	Pre Wash Mass	Post Wash Mass
3/4"	100	0	0
1/2"	89	129	128.3
3/8"	76	282	270.0
#4	52	564	542.4
#8	36	752	734.7
#16	24	893	874.7
#30	15	999	969.2
#50	9	1069	1048.7
#100	7	1093	1073.8
#200	5.1	1115	1091.7
-#200	0	1175	1094.0

$$\text{For No. 4} = \frac{564^2}{542.4} = 586 \text{ g}$$

$$Z_{Ni} = \frac{X^2}{Y}$$

$$\text{For No. 8} = \frac{752^2}{734.7} = 770 \text{ g}$$

3. Estimate Projected Optimum Asphalt Content

3.1 Assuming that no experience with the current sources or contractor is available, the projected optimum and minimum asphalt content will be estimated by both the computational formula and dust/asphalt methods. Refer to Section 7 of the standard for additional information.

b. Computational Formula

$$\begin{aligned} P &= 0.035a + 0.045b + Kc + F \\ &= 0.035 (100 - 36) + 0.045 (36 - 5) + (0.20 \times 5.1) + 0.7 \\ &= 5.4, \text{ round to } 5.5\% \end{aligned}$$

Test specimens will be prepared and tested at 4.5 to 6.5 percent cement contents.

c. Dust/Asphalt Ratio

$$P = \left(\frac{p_{200}}{\text{max. } D / A} \right) = 4.7 / 1.2 = 3.9, \text{ round to } 4.0 \text{ percent}$$

Test specimens will be prepared and tested at 4.0 to 6.0 percent cement contents.

Since the two methods give slightly different ranges, specimens should be prepared and tested at 4.0 to 6.5 percent cement contents.

4. Preparation of Test Specimens

4.1 Thickness Adjustment

The thickness of the trial specimen is 2.48 inches, thus requiring adjustment of the initial aggregate mass by:

$$E_a = \frac{2.5 \times E_i}{H} = \frac{2.5 \times 1175}{2.48} = 1184.5 \text{ g}$$

4.2 Adjust the final batch mass for each sieve by:

$$\text{For No. 4} = \frac{1184.5}{1175} \times \frac{564^2}{542.4} = 591 \text{ g}$$

$$Z_{Na} = \frac{E_a}{E_i} \times Z_{Ni}$$

$$\text{For No. 8} = \frac{1184.5}{1175} \times \frac{752^2}{734.7} = 776 \text{ g}$$

Repeat for the other required sieve sizes; see Table 4 for other sieves.

4.3 Calculate the mass of the asphalt cement for each set of specimens by:

$$\text{for 4.0 percent} = \frac{1184.5 \times 4.0}{100 - 4.0} = 49.4 \text{ g}$$

$$AW = \frac{E_i \text{ (or } E_a) \times P_{bN}}{100 - P_{bN}}$$

$$\text{for 6.5 percent} = \frac{1184.5 \times 6.5}{100 - 6.5} = 82.3 \text{ g}$$

Repeat for the other asphalt contents.

4.4 Calculate the cumulative masses for a maximum specific gravity (Rice) test specimen by:

$$\text{For No. 4} = \frac{2000}{1175} \times 586.5 = 998 \text{ g}$$

$$R_N = \frac{Q}{E_i} \times Z_{Ni}$$

$$\text{For No. 8} = \frac{2000}{1175} \times 770 = 1310$$

Repeat for the other required sieve sizes; see Table 4 for other sieves.

4.5 Coarse Aggregate Properties (such as Specific Gravity, Fracture, Flat-Elongated, Unit Weight, et al)

For each coarse aggregate sieve size, calculate the cumulative mass for the required test specimen(s) of coarse aggregate for the required test procedures by the following formula:

$$C_N = \frac{Q}{\text{No. 4 } R_N} \times R_N$$

$$\text{For CA Specific Gravity for No. 4} = 3000 \text{ g}$$

$$\text{for 1/2"} = \frac{3000}{998} \times 221 = 664 \text{ g}$$

Repeat for the other required sieve sizes, see Table 4 for other sieves.

For Other CA Property Tests substitute the appropriate Q.

4.6 Fine Aggregate Properties (such as Specific Gravity, Sand Equivalent, et al)

For each fine aggregate sieve size, calculate the cumulative masses for the required specimens of fine aggregate specific gravity by the following formula:

$$F_N = \left(\frac{Q}{E_i - Z_{4i}} \right) \times (Z_{Ni} - Z_{4i})$$

$$\text{No. 8} = \left(\frac{1000}{1175.0 - 564} \right) \times (752.0 - 564) = 307 \text{ g}$$

For FA Specific Gravity for

$$\text{No. 200} = \left(\frac{1000}{1175.0 - 564} \right) \times (1115 - 564) = 924.1 \text{ g}$$

Repeat for the other required sieve sizes, See Table 4 for other sieves.

5. Calculations

5.1 Calculate the maximum specific gravity for each asphalt content as follows:

- a. Calculate the effective specific gravity of the aggregate by:

$$G_{se} = \frac{100 - P_b}{\frac{100}{G_{mm}} - \frac{P_b}{G_b}} = \frac{100 - 5.0}{\frac{100}{2.528} - \frac{5.0}{1.009}} = 2.745$$

- b. Calculate the maximum specific gravity for each asphalt content by:

$$G_{mm} = \frac{100}{\frac{100 - P_{bN}}{G_{se}} + \frac{P_{bN}}{G_b}} \quad \text{For 4.0\%} = \frac{100}{\frac{100 - 4.0}{2.745} + \frac{4.0}{1.009}} = 2.568$$

Repeat for other asphalt contents.

5.2 Calculate the percent air voids in total mix (VTM) for each asphalt content by:

$$VTM = \frac{G_{mm} - G_{mb}}{G_{mm}} \times 100 \quad \text{For 4.0\%} = \frac{2.568 - 2.403}{2.568} \times 100 = 6.4$$

5.3 Calculate the percent voids in mineral aggregate (VMA) for each asphalt content by:

- a. Calculate the blended aggregate bulk specific gravity by:

$$G_{sb} = \frac{100}{\frac{P_1}{G_1} + \frac{P_2}{G_2} + \dots + \frac{P_N}{G_N}} = \frac{100}{\frac{50}{2.727} + \frac{50}{2.653}} = 2.689$$

- b. Calculate the percent voids in mineral aggregate for each asphalt content by:

$$VMA = 100 - \frac{G_{mb} (100 - P_b)}{G_{sb}} \quad \text{For 4.0\%} = 100 - \frac{2.403 (100 - 4.0)}{2.689} = 14.2$$

5.4 Calculate the percent voids filled (VFA) with asphalt for each asphalt content by:

$$VFA = 100 \times \frac{VMA - VTM}{VMA} \quad \text{For 4.0\%} = 100 \times \frac{14.2 - 6.4}{14.2} = 55$$

5.5 Calculate the dust/asphalt ratio for each asphalt content by:

- a. Calculate the asphalt absorption by:

$$P_{ba} = 100 \left(\frac{G_{se} - G_{sb}}{G_{sb} \times G_{se}} \right) G_b \quad \text{For 4.0\%} = 100 \left(\frac{2.745 - 2.689}{2.689 \times 2.745} \right) 1.009 = 0.77$$

- b. Calculate the effective asphalt content for each asphalt content by:

$$P_{be} = P_b - \left(\left(\frac{P_{ba}}{100} \right) \times (100 - P_b) \right) \quad \text{For 4.0\%} = 4.0 - \left(\left(\frac{0.77}{100} \right) \times (100 - 4.0) \right) = 3.3$$

- c. Calculate the dust/asphalt ratio by:

$$D/A = \frac{p_{200}}{P_{be}} \quad \text{For } 4.0\% = \frac{4.7}{3.3} = 1.4$$

5.6 Stability:

- c. Correct Stability values for each specimen that differs from the standard 63.5 mm (2.5") thickness by the following:

$$CS = S \times t \quad \text{for Set 1, Specimen 1} = 3145 \times 0.976 = 3070$$

TABLE 4 Cumulative Batch Masses for Example

Sieve Size		Job Mix Formula	Cumulative Mass g					
			Wash Mass	Post Wash	Correction Z _{Ni}	Marshall Z _{Na}	Rice R _N	SG's C _N
25	1	100	0	0				
19	3/4	100	0	0	0	0	0	0
12.5	1/2	89	129	128.3	129.7	130.8	220.8	663.5
9.5	3/8	76	282	270.0	294.5	272.2	501.3	1506.7
4.75	#4	52	564	542.4	586.5	591.2	998.2	3000.0
2.36	#8	36	752	734.7	769.7	775.9	1310.1	311.4
1.18	#16	24	893	874.7	911.7	919.1	1551.8	552.6
0.6	#30	15	999	969.2	1029.7	1038.0	1752.7	753.1
0.3	#50	9	1069	1048.7	1089.7	1098.5	1854.8	855.1
0.15	#100	7	1093	1073.8	1112.5	1121.5	1893.7	893.9
0.075	#200	5.1	1115	1091.7	1138.8	1148.0	1938.4	938.5
-0.075	-200	0	1175		1175	1184.5	2000	1000

Rutting Susceptibility using an Asphalt Pavement Analyzer ATM 419

1. Scope

This method describes a procedure for determining the rut susceptibility of hot mix asphalt using an Asphalt Pavement Analyzer (APA).

2. Apparatus

- Asphalt Pavement Analyzer (APA) – A thermostatically controlled device designed to test the rutting susceptibility of hot mix asphalt by applying repetitive linear loads to compacted test specimens through pressurized hoses.
 - o The APA shall be thermostatically controlled to maintain the test temperature and conditioning chamber at any set point between $30-60 \pm 1^{\circ}\text{C}$ ($85-140 \pm 1^{\circ}\text{F}$).
 - o The APA shall be capable of independently applying loads up to 450 N (100 lbf) to the three wheels. The loads shall be calibrated to the desired test load by a suitable device such as an external force transducer or proving ring.
 - o The pressure in the test hoses shall be adjustable and capable of maintaining pressure up to 830 kPa (120 psi).
 - o The APA shall be capable of testing six cylindrical specimens simultaneously.
 - o The APA shall have a programmable master cycle counter that can be preset to the desired number of cycles for a test. The APA shall be capable to automatically stopping the test at the completion of the programmed number of cycles.
- Balance or scale: Capacity sufficient for the principle sample mass, readable to 0.1 percent or 0.1 g of the total sample mass and meeting the requirements of AASHTO M 231.
- Mixing utensils (bowls, spoon, spatula)
- Ovens and hot plates thermostatically controlled to maintain the various required temperatures within $\pm 3^{\circ}\text{C}$ (5°F).
- Compaction device and molds

3. Test Specimens

Number of test specimens – A sample will consist of six 150 mm diameter x 75 mm (6 in diameter x 3 in) cylindrical specimens.

Production Mix

Samples of plant-produced mixtures shall be obtained in accordance with WAQTC FOP for AASHTO T 168. Samples shall be reduced to the appropriate test size in accordance with WAQTC FOP for AASHTO R 47 and compacted while the mixture is still hot. Reheating of loose plant mixture should be avoided.

Laboratory Prepared Mixtures

Mixture proportions will be batched in accordance to the desired Job Mix Formula. The required batch sizes are determined in accordance to ATM 417, **Preparation of Aggregate and Preparation of Asphalt**. The voids in total mix (VTM) target for the compacted specimens shall be $6.0 + 1.0$ percent unless otherwise directed.

The temperature to which the asphalt binder must be heated to achieve a viscosity of 170 ± 20 cSt ($0.170 + 0.020$ Pa-s) or the mix design mixing temperature shall be the mixing temperature.

Prepare the mixture in accordance with ATM 417, Preparation of Mixtures and Mixture conditioning. The temperature to which the asphalt binder must be heated to achieve a viscosity of 290 ± 30 cSt (0.290 ± 0.030 Pa·s) or the mix design compaction temperature shall be the compaction temperature.

Roadway Core Specimens

Roadway core specimens shall be 150 mm (6 in) outside diameter with all surfaces of the perimeter perpendicular to the surface of the core within 5 mm (3/16 in). Cores shall be trimmed with a wet masonry saw to a height of 75 ± 3 mm ($3 \pm 1/8$ in). Final adjustment of the core to the top of the testing molds shall be done with Plaster of Paris.

4. Compaction of Specimens

1 Superpave Gyratory Compaction

- Apparatus (see AASHTO T 312).
- a. Compaction of the cylindrical specimens with the Superpave Gyratory Compactor will be performed in such a manner so that the target air void content of 6.0 ± 1.0 percent is obtained at the specified height of 75 ± 3 mm.
- b. Remove the mold and base plate from the oven set at the compaction temperature. Place a paper disc in the bottom of the mold assembly.
- c. Transfer the mixture to the mold with care to avoid segregation of the mixture.
- d. Place the mold and mixture in the Superpave Gyratory Compactor and begin compaction as described in the compactor's operation manual.
- e. When the compaction procedure is completed, remove the mold and compacted specimen from the compactor. Extrude the specimen from the mold with care to avoid distorting the specimen until it is cooled.
- f. Compacted specimens should be left at room temperature (about 25°C or 77°F) and allowed to cool overnight.

5. Determining the Voids Total Mix

1. Determine the bulk specific gravity of the test specimens in accordance with WAQTC FOP for AASHTO T 166, Method A.
2. Determine the maximum specific gravity of the test mixture in accordance with WAQTC FOP for AASHTO T 209.
3. Determine the air void contents of the test specimens in accordance with AASHTO T 269.

6. Test Temperature

The test temperature shall be 105°F unless otherwise directed.

7. Initial Measurements

- 2 Place the rut depth measurement template over the specimen. Take initial measurements on three locations of each specimen. Record the measurement for each location to the nearest 0.01 mm.

8. Specimen Conditioning

1. Stabilize the testing chamber temperature at 105°F or as directed.
2. Place the test specimens into the testing molds and secure in the APA.
3. Push the sample holding tray in and secure. Close chamber doors.
4. Allow specimens to condition at the test temperature for 90 minutes.

- 5 Set PRESET COUNTER to 8000 cycles.
- 6 Start the testing. A complete test will take approximately 3.5 hours. At the end of the test cycle, the APA will stop.
- 7 Open the chamber doors, unlock and pull out the sample holding tray.
- 8 Remove specimens from the testing molds and take rut-depth measurements in the same manner as the **Initial Measurements**.

9. Calculations

The rut depth at each location is determined by subtracting the final measurement from the initial measurement.

Determine the average rut depth for each specimen, use the average of all measurements to calculate the average rut depth.

The APA rut depth for the mixture is the average of six cylindrical specimens unless otherwise directed.

10. Report

The test report shall include the following information:

- The laboratory name and date of test.
- The mixture type and description.
- The average rut depth to the nearest 0.1 mm.

This page intentionally left blank.

SAMPLING FRESHLY MIXED CONCRETE

WAQTC TM 2

Scope

This method covers procedures for obtaining representative samples of fresh concrete delivered to the project site and on which tests are to be performed to determine compliance with quality requirements of the specifications under which concrete is furnished. The method includes sampling from stationary, paving and truck mixers, and from agitating and non-agitating equipment used to transport central mixed concrete.

This method also covers the procedure for preparing a sample of concrete for further testing where it is necessary to remove aggregate larger than the designated size for the test method being performed. The removal of large aggregate particles is accomplished by wet sieving.

Sampling concrete may involve hazardous materials, operations, and equipment. This standard does not purport to address all of the safety problems associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices.

Warning—Fresh Hydraulic cementitious mixtures are caustic and may cause chemical burns to skin and tissue upon prolonged exposure.

Apparatus

- Wheelbarrow
- Cover for wheelbarrow (plastic, canvas, or burlap)
- Buckets
- Shovel
- Cleaning equipment: including scrub brush, rubber gloves, water
- Apparatus for wet sieving including a sieve or sieves conforming to AASHTO M 92 of suitable size and conveniently arranged and supported so that the sieve can be shaken rapidly by hand.

Procedure

1. Use every precaution in order to obtain samples representative of the true nature and condition of the concrete being placed being careful not to obtain samples from the very first or very last portions of the batch. The size of the sample will be 1.5 times the volume of concrete required for the specified testing, but not less than 0.03 m^3 (1 ft^3).

Note 1: Sampling should normally be performed as the concrete is delivered from the mixer to the conveying vehicle used to transport the concrete to the forms; however, specifications may require other points of sampling, such as at the discharge of a concrete pump.

- **Sampling from stationary mixers, except paving mixers**

Sample the concrete after a minimum of $1/2 \text{ m}^3$ ($1/2 \text{ yd}^3$) of concrete has been discharged. Perform sampling by passing a receptacle completely through the discharge stream, or by completely diverting the discharge into a sample container.

Take care not to restrict the flow of concrete from the mixer, container, or transportation unit so as to cause segregation. These requirements apply to both tilting and nontilting mixers.

- **Sampling from paving mixers**

Sample after the contents of the paving mixer have been discharged. Obtain material from at least five different locations in the pile and combine into one test sample. Avoid contamination with subgrade material or prolonged contact with absorptive subgrade. To preclude contamination or absorption by the subgrade, the concrete may be sampled by placing a shallow container on the subgrade and discharging the concrete across the container.

- **Sampling from revolving drum truck mixers or agitators**

Sample the concrete after a minimum of $1/2 \text{ m}^3$ ($1/2 \text{ yd}^3$) of concrete has been discharged. Do not obtain samples until after all of the water has been added to the mixer. Do not obtain samples from the very first or last portions of the batch discharge. Sample by repeatedly passing a receptacle through the entire discharge stream or by completely diverting the discharge into a sample container. Regulate the rate of discharge of the batch by the rate of revolution of the drum and not by the size of the gate opening.

- **Sampling from open-top truck mixers, agitators, non-agitating equipment or other types of open-top containers**

Sample by whichever of the procedures described above is most applicable under the given conditions.

- **Sampling from pump or conveyor placement systems**

Sample after a minimum of $1/2 \text{ m}^3$ ($1/2 \text{ yd}^3$) of concrete has been discharged. Do not obtain samples until after all of the pump slurry has been eliminated. Sample by repeatedly passing a receptacle through the entire discharge system or by completely diverting the discharge into a sample container. Do not lower the pump arm from the placement position to ground level for ease of sampling, as it may modify the air content of the concrete being sampled. Do not obtain samples from the very first or last portions of the batch discharge.

2. Transport samples to the place where fresh concrete tests are to be performed and specimens are to be molded. They shall then be combined and remixed with a shovel the minimum amount necessary to ensure uniformity. Protect the sample from direct sunlight, wind, rain, and sources of contamination.
3. Complete test for temperature and start tests for slump and air content within 5 minutes of obtaining the sample. Complete tests as expeditiously as possible. Start molding specimens for strength tests within 15 minutes of obtaining the sample.

Wet Sieving

When required, due to oversize aggregate, the concrete sample shall be wet-sieved, after transporting but prior to remixing, for slump testing, air content testing or molding test specimens, by the following:

1. Place the sieve designated by the test procedure over dampened sample container.
2. Pass the concrete over the designated sieve. Do not overload the sieve (one particle thick).

3. Shake or vibrate the sieve until no more material passes the sieve. A horizontal back and forth motion is preferred.
4. Discard oversize material including all adherent mortar.
5. Repeat until sample of sufficient size is obtained. Mortar adhering to the wet-sieving equipment shall be included with the sample.
6. Remix the sample with a shovel the minimum amount necessary to ensure uniformity.

Note 2: Wet-sieving is not allowed for samples being utilized for density determinations according to the FOP for AASHTO T 121.

This page intentionally left blank.

TEMPERATURE OF FRESHLY MIXED PORTLAND CEMENT CONCRETE

WAQTC FOP FOR AASHTO T 309

Scope

Warning—Fresh Hydraulic cementitious mixtures are caustic and may cause chemical burns to skin and tissue upon prolonged exposure.

This procedure covers the determination of the temperature of freshly mixed portland cement concrete in accordance with AASHTO T 309.

Apparatus

- **Container** — The container shall be made of nonabsorptive material and large enough to provide at least 75 mm (3 in.) of concrete in all directions around the sensor; concrete cover must also be at least three times the nominal maximum size of the coarse aggregate.
- **Temperature Measuring Device** — The temperature measuring device shall be calibrated and capable of measuring the temperature of the freshly mixed concrete to $\pm 0.5^{\circ}\text{C}$ ($\pm 1^{\circ}\text{F}$) throughout the temperature range likely to be encountered. Partial immersion liquid-in-glass thermometers (and possibly other types) shall have a permanent mark to which the device must be immersed without applying a correction factor.
- **Reference Temperature Measuring Device** — The reference temperature measuring device shall be a liquid-in-glass thermometer readable to 0.2°C (0.5°F) that has been verified and calibrated. The calibration certificate or report indicating conformance to the requirements of ASTM E 77 shall be available for inspection.

Calibration of Temperature Measuring Device

Each temperature measuring device shall be verified for accuracy annually and whenever there is a question of accuracy. Calibration shall be performed by comparing readings on the temperature measuring device with another calibrated instrument at two temperatures at least 15°C apart or 27°F apart.

Sample Locations and Times

The temperature of freshly mixed concrete may be measured in the transporting equipment, in forms, or in sample containers, provided the sensor of the temperature measuring device has at least 75 mm (3 in.) of concrete cover in all direction around it.

Complete the temperature measurement of the freshly mixed concrete within 5 minutes of obtaining the sample.

Concrete containing aggregate of a nominal maximum size greater than 75 mm (3 in.) may require up to 20 minutes for the transfer of heat from the aggregate to the mortar after batching.

Procedure

1. Dampen the sample container.
2. Obtain the sample in accordance with the FOP for WAQTC TM 2.
3. Place sensor of the temperature measuring device in the freshly mixed concrete so that it has at least 75 mm (3 in.) of concrete cover in all directions around it.
4. Gently press the concrete in around the sensor of the temperature measuring device at the surface of the concrete so that air cannot reach the sensor.
5. Leave the sensor of the temperature measuring device in the freshly mixed concrete for a minimum of two minutes, or until the temperature reading stabilizes.
6. Complete the temperature measurement of the freshly mixed concrete within 5 minutes of obtaining the sample.
7. Read and record the temperature to the nearest 0.5°C (1°F).

Report

Results shall be reported on standard forms approved for use by the agency. Record the measured temperature of the freshly mixed concrete to the nearest 0.5°C (1°F).

SLUMP OF HYDRAULIC CEMENT CONCRETE

WAQTC FOP FOR AASHTO T 119

Scope

This procedure provides instructions for determining the slump of hydraulic cement concrete in accordance with AASHTO T 119. It is not applicable to non-plastic and non-cohesive concrete. With concrete using 37.5mm (1½ in.) or larger aggregate, the +37.5mm (1½ in.) aggregate must be removed in accordance with the FOP for WAQTC TM 2.

Warning—Fresh Hydraulic cementitious mixtures are caustic and may cause chemical burns to skin and tissue upon prolonged exposure.

Apparatus

- **Mold:** The metal mold shall be provided with foot pieces and handles. The mold must be constructed without a seam. The interior of the mold shall be relatively smooth and free from projections such as protruding rivets. The mold shall be free from dents. A mold that clamps to a rigid nonabsorbent base plate is acceptable provided the clamping arrangement is such that it can be fully released without movement of the mold.
- **Mold:** Other than metal must conform to AASHTO T 119 Sections 5.1.2.1 & 5.1.2.2.
- **Tamping rod:** 16 mm (5/8 in.) diameter and approximately 600 mm (24 in.) long, having a hemispherical tip. (Hemispherical means “half a sphere”; the tip is rounded like half of a ball.)
- **Scoop**
- **Tape measure or ruler** with at least 5 mm or 1/8 in. graduations
- **Base:** Flat, rigid, non-absorbent moistened surface on which to set the slump cone

Procedure

1. Obtain the sample in accordance with FOP for WAQTC TM 2. If any aggregate 37.5mm (1½ in.) or larger is present, aggregate must be removed in accordance with the Wet Sieving portion of the FOP for WAQTC TM 2.

Note 1: Testing shall begin within five minutes of obtaining the sample.

2. Dampen the inside of the cone and place it on a dampened, rigid, nonabsorbent surface that is level and firm.
3. Stand on both foot pieces in order to hold the mold firmly in place.
4. Fill the cone 1/3 full by volume, to a depth of approximately 67 mm (2 5/8 in.) by depth.
5. Consolidate the layer with 25 strokes of the tamping rod, using the rounded end. Distribute the strokes evenly over the entire cross section of the concrete. For this bottom layer, incline the rod slightly and make approximately half the strokes near the perimeter, and then progress with vertical strokes, spiraling toward the center.
6. Fill the cone 2/3 full by volume, to a depth of approximately 155 mm (6 1/8 in.) by depth.

7. Consolidate this layer with 25 strokes of the tamping rod, just penetrating into the bottom layer. Distribute the strokes evenly.
8. Fill the cone to overflowing.
9. Consolidate this layer with 25 strokes of the tamping rod, just penetrating into the second layer. Distribute the strokes evenly. If the concrete falls below the top of the cone, stop, add more concrete, and continue rodding for a total of 25 strokes. Keep an excess of concrete above the top of the mold at all times. Distribute strokes evenly as before.
10. Strike off the top surface of concrete with a screeding and rolling motion of the tamping rod.
11. While holding the filled mold firmly in place, clean overflow concrete away from the base of the mold.
12. Remove the mold from the concrete by raising it carefully in a vertical direction. Raise the mold 300 mm (12 in.) in 5 ± 2 seconds by a steady upward lift with no lateral or torsional (twisting) motion being imparted to the concrete.

The entire operation from the start of the filling through removal of the mold shall be carried out without interruption and shall be completed within an elapsed time of 2 1/2 minutes. Immediately measure the slump by:
13. Invert the slump cone and set it next to the specimen.
14. Lay the tamping rod across the mold so that it is over the test specimen.
15. Measure the distance between the bottom of the rod and the displaced original center of the top of the specimen to the nearest 5 mm (1/4 in.).

Note 2: If a decided falling away or shearing off of concrete from one side or portion of the mass occurs, disregard the test and make a new test on another portion of the sample. If two consecutive tests on a sample of concrete show a falling away or shearing off of a portion of the concrete from the mass of the specimen, the concrete probably lacks the plasticity and cohesiveness necessary for the slump test to be applicable.

16. Discard the tested sample.

Report

Results shall be reported on standard forms approved for use by the agency. Record the slump to the nearest 5 mm (1/4 in.).

DENSITY (UNIT WEIGHT), YIELD, AND AIR CONTENT (GRAVIMETRIC) OF CONCRETE WAQTC FOP FOR AASHTO T 121(See Addendum for DOT&PF Guidelines)

Scope

This procedure covers the determination of density, or unit weight, of freshly mixed concrete in accordance with AASHTO T 121. It also provides formulas for calculating the volume of concrete produced from a mixture of known quantities of component materials, and provides a method for calculating cement content& cementitious material content – the mass of cement or cementitious material per unit volume of concrete. A procedure for calculating water/cement ratio is also covered.

Warning—Fresh Hydraulic cementitious mixtures are caustic and may cause chemical burns to skin and tissue upon prolonged exposure.

Apparatus

- Measure: May be the bowl portion of the air meter used for determining air content under the FOP for AASHTO T 152. Otherwise, it shall be a metal cylindrical container meeting the requirements of AASHTO T 121. The capacity and dimensions of the measure shall conform to those specified in Table 1.
- Balance or scale: Accurate to within 45 g (0.1 lb) or 0.3 percent of the test load, whichever is greater, at any point within the range of use.
- Tamping rod: 16 mm (5/8 in.) diameter and approximately 600 mm (24 in.) long, having a hemispherical tip. (Hemispherical means “half a sphere”; the tip is rounded like half of a ball.)
- Vibrator: 7000 vibrations per minute, 19 to 38 mm (3/4 to 1 1/2 in.) in diameter, and the length of the shaft shall be at least 610 mm (24in).
- Scoop: a receptacle of appropriate size so that each representative increment of the concrete sample can be placed in the container without spillage.
- Strike-off plate: A flat rectangular metal plate at least 6 mm (1/4 in.) thick or a glass or acrylic plate at least 12 mm (1/2 in.) thick, with a length and width at least 50 mm (2 in.) greater than the diameter of the measure with which it is to be used. The edges of the plate shall be straight and smooth within tolerance of 1.5 mm (1/16 in.).
- Mallet: With a rubber or rawhide head having a mass of 0.57 ± 0.23 kg (1.25 ± 0.5 lb) for use with measures of 0.014 m^3 ($1/2 \text{ ft}^3$) or less, or having a mass of 1.02 ± 0.23 kg (2.25 ± 0.5 lb) for use with measures of 0.028 m^3 (1 ft^3).

Table 1
Dimensions of Measures

Capacity m ³ (ft ³)	Inside Diameter mm (in.)	Inside Height mm (in.)	Minimum Thicknesses mm (in.)		Nominal Maximum Size of Coarse Aggregate** mm (in.)
			Bottom	Wall	
0.0071	203 ±2.54	213 ±2.54	5.1	3.0	25
(1/4)*	(8.0 ±0.1)	(8.4 ±0.1)	(0.20)	(0.12)	(1)
0.0142	254 ±2.54	279 ±2.54	5.1	3.0	50
(1/2)	(10.0 ±0.1)	(11.0 ±0.1)	(0.20)	(0.12)	(2)
0.0283	356 ±2.54	284 ±2.54	5.1	3.0	76
(1)	(14.0 ±0.1)	(11.2 ±0.1)	(0.20)	(0.12)	(3)

* Note: Measure may be the base of the air meter used in the FOP for AASHTO T 152.

** Nominal maximum size: One sieve larger than the first sieve to retain more than 10 percent of the material using an agency specified set of sieves based on cumulative percent retained. Where large gaps in specification sieves exist, intermediate sieve(s) may be inserted to determine nominal maximum size.

Calibration of Measure

1. Determine the mass of the dry measure and strike-off plate.
2. Fill the measure with water at a temperature between 16°C and 29°C (60°F and 85°F) and cover with the strike-off plate in such a way as to eliminate bubbles and excess water.
3. Wipe the outside of the measure and cover plate dry, being careful not to lose any water from the measure.
4. Determine the mass of the measure, strike-off plate, and water in the measure.
5. Determine the mass of the water in the measure by subtracting the mass in Step 1 from the mass in Step 4.
6. Measure the temperature of the water and determine its density from Table 2, interpolating as necessary.
7. Calculate the volume of the measure, V_m , by dividing the mass of the water in the measure by the density of the water at the measured temperature, from Table 2.

Table 2
Unit Mass of Water
15°C to 30°C

°C	(°F)	kg/m ³	(lb/ft ³)	°C	(°F)	kg/m ³	(lb/ft ³)
15	(59.0)	999.10	(62.372)	23	(73.4)	997.54	(62.274)
15.6	(60.0)	999.01	(62.366)	23.9	(75.0)	997.32	(62.261)
16	(60.8)	998.94	(62.361)	24	(75.2)	997.29	(62.259)
17	(62.6)	998.77	(62.350)	25	(77.0)	997.03	(62.243)
18	(64.4)	998.60	(62.340)	26	(78.8)	996.77	(62.227)
18.3	(65.0)	998.54	(62.336)	26.7	(80.0)	996.59	(62.216)
19	(66.2)	998.40	(62.328)	27	(80.6)	996.50	(62.209)
20	(68.0)	998.20	(62.315)	28	(82.4)	996.23	(62.192)
21	(69.8)	997.99	(62.302)	29	(84.2)	995.95	(62.175)
21.1	(70.0)	997.97	(62.301)	29.4	(85.0)	995.83	(62.166)
22	(71.6)	997.77	(62.288)	30	(86.0)	995.65	(62.156)

Procedure Selection

There are two methods of consolidating the concrete – rodding and vibration. If the slump is greater than 75 mm (3 in.), consolidation is by rodding. When the slump is 25 to 75 mm (1 to 3 in.), internal vibration or rodding can be used to consolidate the sample, but the method used must be that required by the agency in order to obtain consistent, comparable results. For slumps less than 25 mm (1 in.), consolidate the sample by internal vibration.

Procedure – Rodding

1. Obtain the sample in accordance with the FOP for WAQTC TM 2. Testing may be performed in conjunction with the FOP for AASHTO T 152. When doing so, this FOP should be performed prior to the FOP for AASHTO T 152.

Note 1: If the two tests are being performed using the same sample, this test shall begin within five minutes of obtaining the sample.

2. Determine the mass of the dry empty measure.
3. Dampen the inside of the measure.
4. Fill the measure approximately 1/3 full with concrete.
5. Consolidate the layer with 25 strokes of the tamping rod, using the rounded end. Distribute the strokes evenly over the entire cross section of the concrete. Rod throughout its depth without hitting the bottom too hard.
6. Tap the sides of the measure smartly 10 to 15 times with the mallet to close voids and release trapped air.
7. Add the second layer, filling the measure about 2/3 full.
8. Consolidate this layer with 25 strokes of the tamping rod, penetrating about 25 mm (1 in.) into the bottom layer.
9. Tap the sides of the measure smartly 10 to 15 times with the mallet.
10. Add the final layer, slightly overfilling the measure.

11. Consolidate this layer with 25 strokes of the tamping rod, penetrating about 25 mm (1 in.) into the second layer.

12. Tap the sides of the measure smartly 10 to 15 times with the mallet.

Note 2: The measure should be slightly over full, about 3 mm (1/8 in.) above the rim. If there is a great excess of concrete, remove a portion with the scoop. If the measure is under full, add a small quantity. This adjustment may be done only after consolidating the final layer and before striking off the surface of the concrete.

13. Strike off by pressing the strike-off plate flat against the top surface, covering approximately 2/3 of the measure. Withdraw the strike-off plate with a sawing motion to finish the 2/3 originally covered. Cover the original 2/3 again with the plate; finishing the remaining 1/3 with a sawing motion (do not lift the plate; continue the sawing motion until the plate has cleared the surface of the measure). Final finishing may be accomplished with several strokes with the inclined edge of the strike-off plate. The surface should be smooth and free of voids.

14. Clean off all excess concrete from the exterior of the measure including the rim.

15. Determine and record the mass of the measure and the concrete.

16. If the air content of the concrete is to be determined, proceed to Rodding Procedure Step 13 of the WAQTC FOP for AASHTO T 152.

Procedure - Internal Vibration

1. Perform Steps 1 through 3 of the rodding procedure.

2. Fill the measure approximately half full.

3. Insert the vibrator at four different points in each layer when a 0.0283 m³ (1 ft³) measure is used, and three different points in each layer when a 0.0142 m³ (1/2 ft³), or smaller, measure is used. Do not let the vibrator touch the bottom or sides of the measure.

Note 3: Remove the vibrator slowly, so that no air pockets are left in the material.

Note 4: Continue vibration only long enough to achieve proper consolidation of the concrete. Over vibration may cause segregation and loss of appreciable quantities of intentionally entrained air.

4. Fill the measure a bit over full.

5. Insert the vibrator as in Step 3. Do not let the vibrator touch the sides of the measure, but do penetrate the first layer approximately 25 mm (1 in.).

6. Return to Step 13 of the rodding procedure and continue.

Calculations

- **Density** – Calculate the net mass, M_m , of the concrete in the measure by subtracting the mass of the measure from the gross mass of the measure plus the concrete. Calculate the density, W , by dividing the net mass, M_m , by the volume, V_m , of the measure as shown below.

$$W = \frac{M_m}{V_m}$$

- **Yield** – Calculate the yield, Y , or volume of concrete produced per batch, by dividing the total mass of the batch, W_1 , by the density, W , of the concrete as shown below.

$$Y = \frac{W_1}{W}$$

Note 5: *The total mass, W_1 , includes the masses of the cement, water, and aggregates in the concrete.*

- **Cement Content** – Calculate the actual cement content, N , by dividing the mass of the cement, N_t , by the yield, Y , as shown below.

Note 6: Specifications may require Portland cement content and cementitious materials content

$$N = \frac{N_t}{Y}$$

- **Water Content** – Calculate the mass of water in a batch of concrete by summing the:
 - water added at batch plant
 - water added in transit
 - water added at jobsite
 - free water on coarse aggregate
 - free water on fine aggregate
 - liquid admixtures (if the agency requires this).

This information is obtained from concrete batch tickets collected from the driver. Use the following conversion factors.

To Convert From	To	Multiply By
Liters, L	Kilograms, kg	1.0
Gallons, gal	Kilograms, kg	3.785
Gallons, gal	Pounds, lb	8.34
Milliliters, mL	Kilograms, kg	0.001
Ounces, oz	Milliliters, mL	28.4
Ounces, oz	Kilograms, kg	0.0284
Ounces, oz	Pounds, lb	0.0625
Pounds, lb	Kilograms, kg	0.4536

Calculate the mass of free water on aggregate as follows.

$$\text{Free Water Mass} = \text{Total Aggregate Mass} - \frac{\text{Total Aggregate Mass}}{1 + (\text{Free Water Percentage} / 100)}$$

* To determine Free Water percentage

Total moisture content of the aggregates – absorbed moisture = Free Water

- **Water/Cement Ratio** – Calculate the water/cement ratio by dividing the mass of water in a batch of concrete by the mass of cementitious material in the batch. The masses of the cementitious materials are obtained from concrete batch tickets collected from the driver.

Report

Results shall be reported on standard forms approved for use by the agency and should include the following:

Density (unit weight) to 1 kg/m³ (0.1 lb/ft³)

Yield to 0.01 m³ (0.01 yd³)

Cement content to 1 kg/m³ (1 lb/yd³)

Cementitious material content to 1 kg/m³ (1 lb/yd³)

Water/Cement ratio to 0.01

Addendum WAQTC FOP for AASHTO T 121

Following are guidelines for the use of WAQTC FOP for AASHTO T 121 by the State of Alaska DOT&PF.

1. Under the Heading of Procedure – Rodding, reverse steps 2 and 3.
2. Report the volume of the measure to 0.000001 m³ (0.0001 ft³).

This page intentionally left blank.

AIR CONTENT OF FRESHLY MIXED CONCRETE BY THE PRESSURE METHOD

WAQTC FOP FOR AASHTO T 152 (See Addendum for DOT&PF Guidelines)

Scope

This procedure covers determination of the air content in freshly mixed Portland Cement Concrete containing dense aggregates in accordance with AASHTO T 152, Type B meter. It is not for use with lightweight or highly porous aggregates. This procedure includes calibration of the Type B air meter gauge, and two methods for calibrating the gauge are presented.

Concrete containing aggregate that is 37.5 mm (1 ½ in) or larger must be wet sieved. Sieve a sufficient amount of the sample over the 37.5 mm (1 ½ in) sieve in accordance with the wet sieving portion of the FOP for WAQTC TM 2.

Warning—Fresh Hydraulic cementitious mixtures are caustic and may cause chemical burns to skin and tissue upon prolonged exposure.

Apparatus

- Air meter: Type B, as described in AASHTO T 152
- Balance or scale: Accurate to 0.3 percent of the test load at any point within the range of use (for Method 1 calibration only)
- Tamping rod: 16 mm (5/8 in) diameter and approximately 600 mm (24 in) long, having a hemispherical tip. (Hemispherical means “half a sphere”; the tip is rounded like half of a ball.)
- Vibrator: 7000 vibrations per minute, 19 to 38 mm (0.75 to 1.50 in) in diameter, at least 75 mm (3 in) longer than the section being vibrated for use with low slump concrete
- Scoop: a receptacle of appropriate size so that each representative increment of the concrete sample can be placed in the container without spillage.
- Container for water: rubber syringe (may also be a squeeze bottle)
- Strike-off bar: Approximately 300 mm × 22 mm × 3 mm (12 in × 3/4 in × 1/8 in)
- Strike-off plate: A flat rectangular metal plate at least 6 mm (1/4 in.) thick or a glass or acrylic plate at least 12 mm (1/2 in.) thick, with a length and width at least 50 mm (2 in.) greater than the diameter of the measure with which it is to be used. The edges of the plate shall be straight and smooth within tolerance of 1.5 mm (1/16 in.).

Note 1: Use either the strike-off bar or strike-off plate; both are not required.

- Mallet: With a rubber or rawhide head having a mass of 0.57 ±0.23 kg (1.25 ±0.5 lb)

Calibration of Air Meter Gauge

Note 2: There are two methods for calibrating the air meter, mass or volume.

1. Screw the short piece of straight tubing into the threaded petcock hole on the underside of the cover. Determine the mass of the dry, empty air meter bowl and cover assembly (mass method only).
2. Fill the bowl nearly full with water.
3. Clamp the cover on the bowl with the tube extending down into the water. Mark the petcock with the tube attached for future reference.
4. Add water through the petcock having the pipe extension below until all air is forced out the other petcock. Rock the meter slightly until all air is expelled through the petcock.
5. Wipe off the air meter bowl and cover assembly, and determine the mass of the filled unit (Mass Method only).
6. Pump up the air pressure to a little beyond the predetermined initial pressure indicated on the gauge. Wait a few seconds for the compressed air to cool, and then stabilize the gauge hand at the proper initial pressure by pumping up or relieving pressure, as needed.
7. Close both petcocks and immediately open the main air valve exhausting air into the bowl. Wait a few seconds until the meter needle stabilizes. The gauge should now read 0 percent. If two or more tests show a consistent variation from 0 percent in the result, change the initial pressure line to compensate for the variation, and use the newly established initial pressure line for subsequent tests.
8. Determine which petcock has the straight tube attached to it. Attach the curved tube to external portion of the same petcock.
9. Pump air into the air chamber. Open the petcock with the curved tube attached to it. Open the main air valve for short periods of time until 5 percent of water by mass or volume has been removed from the air meter. Remember to open both petcocks to release the pressure in the bowl and drain the water in the curved tube back into the bowl. To determine the mass of the water to be removed, subtract the mass found in Step 1 from the mass found in Step 5. Multiply this value by 0.05. This is the mass of the water that must be removed. To remove 5 percent by volume, remove water until the external calibration vessel is level full.

Note 3: Many air meters are supplied with a calibration vessel(s) of known volume that are used for this purpose. Calibration vessel(s) should be brass, not plastic, and must be protected from crushing or denting. If an external calibration vessel is used, confirm what percentage volume it represents for the air meter being used. Vessels commonly represent 5 percent volume, but they are for specific size meters. This should be confirmed by mass.

10. Remove the curved tube. Pump up the air pressure to a little beyond the predetermined initial pressure indicated on the gauge. Wait a few seconds for the compressed air to cool, and then stabilize the gauge hand at the proper initial pressure by pumping up or relieving pressure, as needed.
11. Close both petcocks and immediately open the main air valve exhausting air into the bowl. Wait a few seconds until the meter needle is stabilized. The gauge should now read 5.0 ± 0.1 percent. If the gauge is outside that range, the meter needs adjustment. The adjustment could involve adjusting the starting point so that the gauge reads 5.0 ± 0.1 percent when this calibration is run, or could involve moving the gauge needle to read 5.0 percent. Any adjustment should comply with the manufacturer's recommendations.

Note 4: Calibration shall be performed at the frequency required by the agency. Record the date of the calibration, the calibration results, and the name of the technician performing the calibration in the log book kept with each air meter.

12. When the gauge hand reads correctly at 5.0 percent, additional water may be withdrawn in the same manner to check the results at other values such as 10 percent or 15 percent.
13. If an internal calibration vessel is used, follow steps 1 through 8 to set initial reading.
14. Release pressure from the bowl and remove cover. Place the internal calibration vessel into the bowl. This will displace 5 percent of the water in the bowl. (See AASHTO T 152 for more information on internal calibration vessels.)
15. Place the cover back on the bowl and add water through the petcock until all the air has been expelled.
16. Pump up the air pressure chamber to the initial pressure. Wait a few seconds for the compressed air to cool, and then stabilize the gauge hand at the proper initial pressure by pumping up or relieving pressure, as needed.
17. Close both petcocks and immediately open the main air valve exhausting air into the bowl. Wait a few seconds until the meter needle stabilizes. The gauge should now read 5 percent.

Note 5: Remove the extension tubing from threaded petcock hole in the underside of the cover before starting the test procedure.

Procedure Selection

There are two methods of consolidating the concrete – rodding and vibration. If the slump is greater than 75 mm (3 in.), consolidation is by rodding. When the slump is 25 to 75 mm (1 to 3 in.), internal vibration or rodding can be used to consolidate the sample, but the method used must be that required by the agency in order to obtain consistent, comparable results. For slumps less than 25 mm (1 in.), consolidate the sample by internal vibration.

Procedure – Rodding

1. Obtain the sample in accordance with the FOP for WAQTC TM 2. If any aggregate 37.5mm (1½ in.) or larger is present, aggregate must be removed in accordance with the Wet Sieving portion of the FOP for WAQTC TM 2.

Note 6: Testing shall begin within five minutes of obtaining the sample.

2. Dampen the inside of the air meter bowl and place on a firm level surface.
3. Fill the bowl approximately 1/3 full with concrete.
4. Consolidate the layer with 25 strokes of the tamping rod, using the rounded end. Distribute the strokes evenly over the entire cross section of the concrete. Rod throughout its depth without hitting the bottom too hard.
5. Tap the sides of the bowl smartly 10 to 15 times with the mallet to close voids and release trapped air.
6. Add the second layer, filling the bowl about 2/3 full.
7. Consolidate this layer with 25 strokes of the tamping rod, penetrating about 25 mm (1 in.) into the bottom layer.
8. Tap the sides of the bowl 10 to 15 times with the mallet.
9. Add the final layer, slightly overfilling the bowl.

10. Consolidate this layer with 25 strokes of the tamping rod, penetrating about 25 mm (1 in.) into the second layer.
11. Tap the sides of the bowl smartly 10 to 15 times with the mallet.

Note 7: The bowl should be slightly over full, about 3 mm (1/8 in.) above the rim. If there is a great excess of concrete, remove a portion with the trowel or scoop. If the bowl is under full, add a small quantity. This adjustment may be done only after consolidating the final layer and before striking off the surface of the concrete.
12. Strike off the surface of the concrete and finish it smoothly with a sawing action of the strike-off bar or plate, using great care to leave the bowl just full. The surface should be smooth and free of voids.
13. Clean the top flange of the bowl to ensure a proper seal.
14. Moisten the inside of the cover and check to see that both petcocks are open and the main air valve is closed.
15. Clamp the cover on the bowl.
16. Inject water through a petcock on the cover until water emerges from the petcock on the other side.
17. Incline slightly and gently rock the air meter until no air bubbles appear to be coming out of the second petcock. The petcock expelling water should be higher than the petcock where water is being injected. Return the air meter to a level position and verify that water is present in both petcocks.
18. Close the air bleeder valve and pump air into the air chamber until the needle goes past the initial pressure determined for the gauge. Allow a few seconds for the compressed air to cool.
19. Tap the gauge gently with one hand while slowly opening the air bleeder valve until the needle rests on the initial pressure. Close the air bleeder valve.
20. Close both petcocks.
21. Open the main air valve.
22. Tap the sides of the bowl smartly with the mallet.
23. With the main air valve open, lightly tap the gauge to settle the needle, and then read the air content to the nearest 0.1 percent.
24. Release or close the main air valve.
25. Open both petcocks to release pressure, remove the concrete, and thoroughly clean the cover and bowl with clean water.
26. Open the main air valve to relieve the pressure in the air chamber.

Procedure - Internal Vibration

1. Obtain the sample in accordance with the FOP for WAQTC TM 2. If any aggregate 37.5mm (1½ in.) or larger is present, aggregate must be removed in accordance with the Wet Sieving portion of the FOP for WAQTC TM 2.
2. Dampen the inside of the air meter bowl and place on a firm level surface.
3. Fill the bowl approximately half full.
4. Insert the vibrator at three different points. Do not let the vibrator touch the bottom or sides of the bowl.

Note 8: Remove the vibrator slowly, so that no air pockets are left in the material.

Note 9: Continue vibration only long enough to achieve proper consolidation of the concrete. Over vibration may cause segregation and loss of appreciable quantities of intentionally entrained air.

5. Fill the bowl a bit over full.
6. Insert the vibrator as in Step 4. Do not let the vibrator touch the sides of the bowl, and penetrate the first layer approximately 25 mm (1 in.).
7. Return to Step 12 of the rodding procedure and continue.

Report

- Results shall be reported on standard forms approved for use by the agency.
- Record the percent of air to the nearest 0.1 percent.
- Some agencies require an aggregate correction factor in order to determine total percent entrained air.

Total percent entrained air = Gauge reading – aggregate correction factor from mix design

(See AASHTO T 152 for more information.)

Addendum WAQTC FOP for AASHTO T 152

Following are guidelines for the use of WAQTC FOP for AASHTO T 152 by the State of Alaska DOT&PF.

1. An alternate calibration procedure may be used as found in Standard Practice 8.
2. Correction Factors should be checked for each new aggregate source and for sources that have a history of a correction factor in excess of 0.4 percent.
3. For concrete with a slump equal to or greater than 1 in, the concrete shall be rodded.

MAKING AND CURING CONCRETE TEST SPECIMENS IN THE FIELD

WAQTC FOP FOR AASHTO T 23 (See Addendum for DOT&PF Guidelines)

Scope

This procedure covers the method for making, initially curing, and transporting concrete test specimens in the field in accordance with AASHTO T 23.

Warning—Fresh Hydraulic cementitious mixtures are caustic and may cause chemical burns to skin and tissue upon prolonged exposure.

Apparatus and Test Specimens

- Concrete cylinder molds: Conforming to AASHTO M 205 with a length equal to twice the diameter. Standard specimens shall be 150 mm (6 in.) by 300 mm (12 in.) cylinders. Mold diameter must be at least three times the maximum aggregate size unless wet sieving is conducted according to the FOP for WAQTC TM 2. Agency specifications may allow cylinder molds of 100 mm (4 in.) by 200 mm (8 in.) when the nominal maximum aggregate size does not exceed 25 mm (1 in.).
- Beam molds: Rectangular in shape with ends and sides at right angles to each other. Must be sufficiently rigid to resist warpage. Surfaces must be smooth. Molds shall produce length no more than 1.6 mm (1/16 in.) shorter than that required (greater length is allowed). Maximum variation from nominal cross section shall not exceed 3.2 mm (1/8 in.). Ratio of width to depth may not exceed 1:5; the smaller dimension must be at least 3 times the maximum aggregate size. Unless otherwise noted in specifications, beam molds for casting specimens in the field shall result in specimens having width and depth of not less than 150 mm (6 inches). Specimens shall be cast and hardened with the long axes horizontal.
- Standard tamping rod: 16 mm (5/8 in.) in diameter and approximately 600 mm (24 in.) long, having a hemispherical tip for preparing 150mm (6 in.) x 300 mm (12 in.) cylinders.
- Small tamping rod: 10 mm (3/8 in.) diameter and approximately 305 mm (12 in.) long, having a hemispherical tip for preparing 100 mm (4 in.) x 200 mm (8 in.) cylinders.
- Vibrator: At least 7000 vibrations per minute, with a diameter no more than ¼ the diameter or width of the mold and at least 75 mm (3 in.) longer than the section being vibrated for use with low slump concrete.
- Scoop: a receptacle of appropriate size so that each representative increment of the concrete sample can be placed in the container without spillage.
- Trowel or float
- Mallet: With a rubber or rawhide head having a mass of 0.57 ± 0.23 kg (1.25 ± 0.5 lb.).
- Rigid base plates and cover plates: may be metal, glass, or plywood.
- Initial curing facilities: Temperature-controlled curing box or enclosure capable of maintaining the required range of 16 to 27°C (60 to 80°F) during the entire initial curing period. (fFor concrete with compressive strength of 40 Mpa (6000 psi) or more, the temperature shall be 20 to 26°C (68 to 78°F). As an alternative, sand or earth for initial cylinder protection may be used provided that the required temperature range is maintained and the specimens are not damaged.

- Thermometer: Capable of registering both maximum and minimum temperatures during the initial cure.

Procedure – Making Specimens – General

1. Obtain the sample according to the FOP for WAQTC TM 2.
2. Wet Sieving per the FOP for WAQTC TM 2 is required for:
 - a) 150 mm (6 in.) diameter specimens containing aggregate with a nominal maximum size greater than 50 mm (2 in.); screen the sample over the 37.5 mm (1½ in.) sieve.
 - b) 100 mm (4 in.) diameter specimens containing aggregate with a nominal maximum size greater than 25 mm (1 in.); screen the sample over the 25 mm (1 in.) sieve.
3. Remix the sample after transporting to testing location.
4. Begin making specimens within 15 minutes of obtaining the sample.
5. Set molds upright on a level, rigid base in a location free from vibration and relatively close to where they will be stored.
6. Fill molds in the required number of layers, attempting to slightly overfill the mold on the final layer. Add or remove concrete prior to completion of consolidation to avoid a deficiency or excess of concrete.
7. There are two methods of consolidating the concrete – rodding and internal vibration. If the slump is greater than 25 mm (1 in.), consolidation may be by rodding or vibration. When the slump is 25 mm (1 in.) or less, consolidate the sample by internal vibration. Agency specifications may dictate when rodding or vibration will be used.

Procedure – Making Cylinders – Rodding

1. For the standard 150 mm (6 in.) by 300 mm (12 in.) specimen, fill each mold in three approximately equal layers, moving the scoop or trowel around the perimeter of the mold to evenly distribute the concrete. For the 100 mm (4 in.) by 200 mm (8 in.) specimen, fill the mold in two layers. When filling the final layer, slightly overfill the mold.
2. Consolidate each layer with 25 strokes of the appropriate tamping rod, using the rounded end. Distribute strokes evenly over the cross section of the concrete. Rod the first layer throughout its depth without forcibly hitting the bottom. For subsequent layers, rod the layer throughout its depth penetrating approximately 25 mm (1 in.) into the underlying layer.
3. After rodding each layer, tap the sides of each mold 10 to 15 times with the mallet (reusable steel molds) or lightly with the open hand (single-use light-gauge molds).
4. Strike off the surface of the molds with tamping rod or straightedge and begin initial curing.

Note 1: Floating or troweling is permitted instead of striking off with rod or straightedge.

Procedure – Making Cylinders – Internal Vibration

1. Fill the mold in two layers.
2. Insert the vibrator at the required number of different points for each layer (two points for 150 mm (6 in.) diameter cylinders; one point for 100 mm (4 in.) diameter cylinders). When vibrating the bottom layer, do not let the vibrator touch the bottom or sides of the mold. When vibrating the top layer, the vibrator shall penetrate into the underlying layer approximately 25 mm (1 in.)
3. Remove the vibrator slowly, so that no large air pockets are left in the material.

Note 2: Continue vibration only long enough to achieve proper consolidation of the concrete. Over vibration may cause segregation and loss of appreciable quantities of intentionally entrained air.

4. After vibrating each layer, tap the sides of each mold 10 to 15 times with the mallet (reusable steel molds) or lightly with the open hand (single-use light-gauge molds).
5. Strike off the surface of the molds with tamping rod or straightedge and begin initial curing.

Procedure – Making Flexural Beams – Rodding

1. Fill the mold in two approximately equal layers with the second layer slightly overfilling the mold.
2. Consolidate each layer with the tamping rod once for every 1300 mm² (2 in²) using the rounded end. Rod each layer throughout its depth, taking care to not forcibly strike the bottom of the mold when compacting the first layer. Rod the second layer throughout its depth, penetrating approximately 25 mm (1 in.) into the lower layer.
3. After rodding each layer, strike the mold 10 to 15 times with the mallet and spade along the sides and end using a trowel.
4. Strike off to a flat surface using a float or trowel and begin initial curing.

Procedure – Making Flexural Beams – Vibration

1. Fill the mold to overflowing in one layer.
2. Consolidate the concrete by inserting the vibrator vertically along the centerline at intervals not exceeding 150 mm (6 in.). Take care to not over-vibrate, and withdraw the vibrator slowly to avoid large voids. Do not contact the bottom or sides of the mold with the vibrator.
3. After vibrating, strike the mold 10 to 15 times with the mallet.
4. Strike off to a flat surface using a float or trowel and begin initial curing.

Procedure – Initial Curing

- When moving cylinder specimens made with single use molds support the bottom of the mold with trowel, hand, or other device.
- For initial curing of cylinders, there are two methods, use of which depends on the agency. In both methods, the curing place must be firm, within ¼ in. of a level surface, and free from vibrations or other disturbances.
- Maintain initial curing temperature of 16 to 27° C (60 to 80°F) or 20 to 26°C (68 to 78°F) for concrete with strength of 40 Mpa (6000 psi) or more.

- Prevent loss of moisture.

Method 1 – Initial cure in a temperature controlled chest-type curing box

1. Finish the cylinder using the tamping rod, straightedge, float, or trowel. The finished surface shall be flat with no projections or depressions greater than 3.2 mm (1/8 in.).
2. Place the mold in the curing box. When lifting light-gauge molds be careful to avoid distortion (support the bottom, avoid squeezing the sides).
3. Place the lid on the mold to prevent moisture loss.
4. Mark the necessary identification data on the cylinder mold and lid.

Method 2 – Initial cure by burying in earth or by using a curing box over the cylinder

Note 3: This procedure may not be the preferred method of initial curing due to problems in maintaining the required range of temperature.

1. Move the cylinder with excess concrete to the initial curing location.
2. Mark the necessary identification data on the cylinder mold and lid.
3. Place the cylinder on level sand or earth, or on a board, and pile sand or earth around the cylinder to within 50 mm (2 in.) of the top.
4. Finish the cylinder using the tamping rod, straightedge, float, or trowel. Use a sawing motion across the top of the mold. The finished surface shall be flat with no projections or depressions greater than 3.2 mm (1/8 in.).
5. If required by the agency, place a cover plate on top of the cylinder and leave it in place for the duration of the curing period, or place the lid on the mold to prevent moisture loss.

Procedure – Transporting Specimens

- After 24 to 48 hours of initial curing, the specimens will be transported to the laboratory for a final cure. Specimen identity will be noted along with the date and time the specimen was made and the maximum and minimum temperatures registered during the initial cure.
- While in transport, specimens shall be protected from jarring, extreme changes in temperature, freezing, or moisture loss.
- Cylinders shall be secured so that the axis is vertical.
- Transportation time shall not exceed 4 hours.

Final Curing

- Upon receiving cylinders at the laboratory, remove the cylinder from the mold and apply the appropriate identification.
- For all specimens (cylinders or beams), final curing must be started within 30 minutes of mold removal. Temperature shall be maintained at $23^{\circ} \pm 2^{\circ}\text{C}$ ($73 \pm 3^{\circ}\text{F}$). Free moisture must be present on

the surfaces of the specimens during the entire curing period. Curing may be accomplished in a moist room or water tank conforming to AASHTO M 201.

- For cylinders, during the final 3 hours prior to testing the temperature requirement may be waived, but free moisture must be maintained on specimen surfaces at all times until tested.
- Final curing of beams must include immersion in lime-saturated water for at least 20 hours prior to testing.

Report

- Report on standard agency forms.
- Pertinent placement information for identification of project, element(s) represented, etc.
- Date and time molded.
- Test ages.
- Slump, air content, & density.
- Temperature (concrete, initial cure max. & min., and ambient).
- Method of initial curing.
- Other information as required by agency, such as: concrete supplier, truck number, invoice number, water added, etc.

Addendum WAQTC FOP for AASHTO T 23

Following are guidelines for the use of WAQTC FOP for AASHTO T 23 by the State of Alaska DOT&PF.

1. If the slump is 1 in or less, consolidate by vibrator. If the slump is above 1 in, consolidate by rodding. Concrete for curb and gutter shall be rodded regardless of slump.
2. When cylinders must be transported, transportation time shall not exceed 8 hours. If this transportation time requirement cannot be met, the transportation time must be approved by the Engineer in writing prior to transporting.
3. Acceptance testing may be done with either 150 mm by 300 mm (6 in by 12 in) cylinders or 100 mm by 200 mm (4 in by 8 in) cylinders.

Field Sampling and Fabrication of 50 mm (2 in) Cube Specimens using Grout (Non-Shrink) and or Mortar WAQTC TM 12 (See Addendum for DOT&PF Guidelines)

1 Scope

- 1.1 This method covers field sampling and fabrication and initial curing of 50 mm (2 in) cube specimens of non-shrink grout and/or mortar materials.
- 1.2 The values stated in either SI or inch-pound units shall be regarded separately as standard. The inch-pound units are shown in brackets. The values stated might not be exact equivalents; therefore, each system must be used independently of the other.

Note 1—Unit weight was the previous terminology used to describe the property determined by this test method, which is mass per unit volume.

- 1.3 The text of this test method references notes and footnotes that provide explanatory information. These notes and footnotes (excluding those in tables) shall not be considered as requirements of this test method.
- 1.4 *This standard does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use. Warning—Fresh hydraulic cementitious mixtures are caustic and may cause chemical burns to skin and tissue upon prolonged exposure.*

2 Referenced Documents

2.1 AASHTO / ASTM

- C 1107 Standard Specification for Packaged Dry, Hydraulic-Cement Grout (Non-shrink)
- T 106 / C 109 Test method for Compressive Strength of Hydraulic Cement Mortars (Using 2 in. or 50 mm Cube Specimens.)

3 Apparatus

- 3.1 Specimen Molds including cover plate (s): The 2 in. (50 mm) cube specimen molds shall be tight fitting and made of brass or other suitable material. This material shall not be susceptible to attack by the cement mortar. The molds shall have not more than three (3) cube compartments and shall be separable into not more than two (2) parts. The parts of the molds, when assembled, shall be positively held together. The cover plate(s) working surface shall be plane and shall be positively attached to the side walls of the mold. The interior faces of the molds shall conform to the tolerances of table 1.

Table 1

Permissible Variations of Specimen Molds				
	2 in. Cube Molds		50 mm Cube Molds	
Parameter	New	In Use	New	In Use
Planeness of Sides	<0.001 in.	<0.002 in.	<0.025 mm	<0.05 mm
Distance Between Opposite Sides	2 in. \pm 0.005 in.	2 in. \pm 0.02 in.	50 mm \pm 0.13 mm	50 mm \pm 0.50 mm
Height of Each Compartment	2 in. + 0.01 in. to -0.005 in.	2 in + 0.01 in. to -0.015 in.	50 mm + 0.25 mm to -0.13 mm	50 mm + 0.25 mm to -0.38 mm
Angle Between Adjacent Faces ^A	90 \pm 0.5°	90 \pm 0.5°	90 \pm 0.5°	90 \pm 0.5°

^AMeasured at points slightly removed from the intersection. Measured separately for each compartment between all the interior faces and the adjacent face and between interior faces and top and bottom planes of the mold.

- 3.2 Tamper: A non-absorptive, nonabrasive, non-brittle material such as a hard rubber compound having a Shore A durometer hardness of 80 ± 10 . The tamper shall have a cross section of about 1/2 in. x 1 in. (13 mm x 25 mm) and a length of 5 in. to 6 in. (125 mm to 150 mm). The tamping face shall be flat and at right angles to the length of the tamper.
- 3.3 Trowel: Steel bladed 100 to 150 mm (4 in to 6 in) in length, with straight edges.
- 3.4 Water tight container: a 150 mm x 300 mm (6 in x 12 in) concrete cylinder mold with lid
- 3.5 Other Equipment: Rubber gloves, scoop, clamps to secure the cover plate, light release oil for oiling the molds, small brush or lint-free cloth for applying and removing excess release oil, burlap or wrapping cloth capable of retaining moisture.

4 Sampling

- 4.1 Samples shall be obtained in accordance with WAQTC TM 2 when the batch equals or exceeds 1 m³ (1 cy). When the batch is less than 1 m³ (1 cy) sample from the batch after discharge. If remixing is required sample after remixing. Begin molding the specimens within an elapsed time of not more than 2 1/2 minutes from completion of the mixing.
- 4.2 Obtain a representative sample of the mix. Samples shall be a minimum size of 2000 g (4 lb) for each set of three (3) cubes to be fabricated.

5 Procedure


- 5.1 Assemble both portions of the mold and the bottom cover plate. All joints shall be water tight. If not water tight, seal the surfaces where the halves of the mold join by applying a coating of light cup grease(non water soluble). The amount should be sufficient to extrude slightly when the halves are tightened together. Repeat this process for attaching the mold to the bottom cover plate. Remove any excess grease. Apply a thin coating of release agent to the interior faces of the mold and the bottom cover plate. Wipe the mold faces and base plate as necessary to remove any excess release agent and to achieve a thin, even coating on the interior surfaces. Adequate

coating is that which is just sufficient to allow a distinct fingerprint to remain following light finger pressure.


- 5.2 Place a layer of grout about 25 mm (1 in) (approximately one-half of the depth of the mold) in all of the cube compartments. Consolidate according to the consistency (plastic or fluid) of the mix.
 - 5.2.1. For plastic mixes, tamp the lift in four rounds of 8 tamps for a total of 32 tamps with the rubber tamper in 10 seconds. See [Figure 1](#) for tamping sequence of each round. Rounds 1 and 3; and 2 and 4 shall be the same.
 - 5.2.2. For fluid mixes, puddle the lift 5 times with a gloved finger. See [Figure 2](#) for tamping sequence.
- 5.3 Place the second lift in each of the cube compartments, slightly over-filling each compartment. Consolidate the material in the same fashion as the first lift with the additional requirement that during consolidation of the second lift any grout forced out onto the top of the mold after each round will be pushed back onto the compartment by means of the tamper and/or gloved fingers before the next consolidation round. When consolidation of the grout is completed, material should extend slightly above the top of the mold. Push any grout forced out onto the top of the mold after the last round back onto the compartment with the trowel.
- 5.4 Smooth off the cubes by drawing the flat side of the trowel (with the leading edge slightly raised) once across the top of each cube at right angles to the length of the mold. Then, for the purpose of leveling the mortar and making the mortar that protrudes above the top of the mold of more uniform thickness, draw the flat trailing edge of the trowel (with leading edge slightly raised) once lightly along the length of the mold. Cut off the mortar to a plane surface flush with the top of the mold by drawing the straight edge of the trowel (held nearly perpendicular to the mold) with a sawing motion over the length of the mold. The material shall be flush with the top of the mold.
- 5.5 Immediately secure the top cover plate to the cube mold.
- 5.6 Place the molds in a secure location away from vibration and as close as possible to the structure for initial curing. Cover with wet burlap, towels, or rags, seal it in a plastic sack in a level location out of direct sunlight, and record the time. These samples shall remain undisturbed and protected from freezing or overheating for a period of 24 ± 4 hours.
- 5.7 At the end of the initial curing period as required by the agency either;
 - 5.7.1. Place the sealed plastic sack into a water tight container. Transport the cube samples immediately to the location of final curing. During transport, the cube samples shall be protected from jarring, freezing, and moisture loss.
 - 5.7.2. Disassemble the mold and carefully remove the cube samples. Using a permanent marker, identify the cube samples. Handling the cube samples very carefully, wrap them in wet burlap or wet towels and place them into a water tight container. Transport the cube samples immediately to the location of final curing. During transport, the cube samples shall be protected from jarring, freezing, and moisture loss.
- 5.8 Final curing shall consist of immersing the cube samples in a lime-saturated water storage tank. They are to remain in the storage tank until time of test. (Curing cube samples of material other

than hydraulic cement shall be in conformance with the manufacturer's recommendations.) The storage tank shall be made of non-corroding materials.

FIGURE # 1

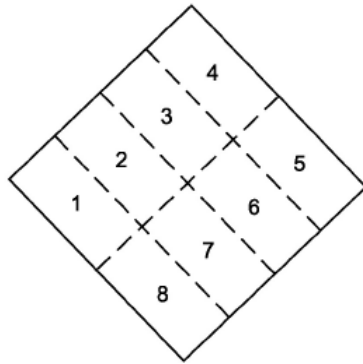


Rounds 1 and 3

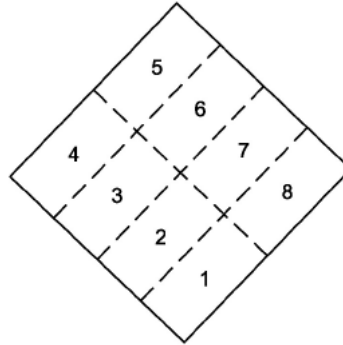

Rounds 2 and 4

FIGURE # 2

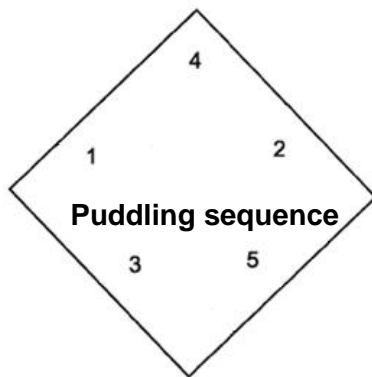

Addendum WAQTC TM 12

Following are guidelines for the use of WAQTC TM 12 by the State of Alaska DOT&PF.

1. Terminology:
 - a. Plastic mix is defined as material viscous enough that an indentation will be left in the surface of the grout after tamping.
 - b. Fluid mix is defined as material fluid enough that little or no indentation will be left in the surface of the grout after puddling.
2. Three specimens shall be cast for each test age required.
3. Applicable sections of AASHTO T 106 shall be followed for final curing, testing compressive strength and reporting test results.

This page intentionally left blank.

Terminology SP 1

1. Scope

This standard practice provides terminology as interpreted and defined by the State of Alaska. The definitions of the American Association of State Highway and Transportation Officials (AASHTO) are the ones most commonly followed by this Agency.

Absorption – The increase in the mass of aggregate due to water being absorbed into the pores of the material, but not including water adhering to the outside surface of the particles, expressed as a percentage of the dry mass.

Acceptance sampling and testing– Sampling and testing performed by the State of Alaska, or its designated agent, to evaluate acceptability of the final product. This is also called verification sampling and testing when specifically used to validate the contractor's data.

Admixture – Material other than water, cement, and aggregates in portland cement concrete (PCC).

Aggregate – Hard granular material of mineral composition, including sand, gravel, slag or crushed stone, used in roadway base and in Portland Cement Concrete (PCC) and Asphalt concrete pavement.

- **Coarse aggregate** – Aggregate retained on or above the 4.75 mm (No. 4) sieve.
- **Coarse-graded aggregate** – Aggregate having a predominance of coarse sizes.
- **Dense-graded aggregate** – Aggregate having a particle size distribution such that voids occupy a relatively small percentage of the total volume.
- **Fine aggregate** – Aggregate passing the 4.75 mm (No. 4) sieve.
- **Fine-graded aggregate** – Aggregate having a predominance of fine sizes.
- **Mineral filler** – A fine mineral product at least 70 percent of which passes a 75 μ m (No. 200) sieve.
- **Open-graded gap-graded aggregate** – Aggregate having a particle size distribution such that voids occupy a relatively large percentage of the total volume.
- **Well-Graded Aggregate** – Aggregate having an even distribution of particle sizes.

Aggregate storage bins – Bins that store aggregate for feeding material to the dryer in an asphalt concrete pavement plant in substantially the same proportion as required in the finished mix.

Agitation – Provision of gentle motion in Portland Cement Concrete (PCC) sufficient to prevent segregation and loss of plasticity.

Air voids – Total volume of the small air pockets between coated aggregate particles in asphalt concrete pavement; expressed as a percentage of the bulk volume of the compacted paving mixture.

Ambient temperature – Temperature of the surrounding air.

Angular aggregate – Aggregate possessing well-defined edges at the intersection of roughly planar faces.

Apparent specific gravity – The ratio of the mass, in air, of a volume of the impermeable portion of aggregate to the mass of an equal volume of water.

Asphalt – A dark brown to black cementitious material in which the predominate constituents are bitumens occurring in nature or obtained through petroleum processing. Asphalt is a constituent of most crude petroleum.

Asphalt cement – Asphalt specially prepared in quality and consistency for use in the manufacture of Hot Mix Asphalt (HMA) pavement.

Asphalt concrete batch plant – A manufacturing facility for producing asphalt concrete that proportions aggregate by weight and asphalt by weight or volume.

Asphalt concrete continuous mix plant – A manufacturing facility for producing asphalt concrete that proportions aggregate and asphalt by a continuous volumetric proportioning system without specific batch intervals.

Automatic cycling control – A control system in which the opening and closing of the weigh hopper discharge gate, the bituminous discharge valve, and the pug mill discharge gate are actuated by means of automatic mechanical or electronic devices without manual control. The system includes preset timing of dry and wet mixing cycles.

Automatic dryer control – A control system that automatically maintains the temperature of aggregates discharged from the dryer.

Automatic proportioning control – A control system in which proportions of the aggregate and asphalt fractions are controlled by means of gates or valves that are opened and closed by means of automatic mechanical or electronic devices without manual control.

Bag (of cement) – 94 lb of portland cement. (Approximately 1 ft³ of bulk cement.)

Base – A layer of selected material constructed on top of subgrade or subbase and below the paving on a roadway.

Bias – The offset or skewing of data or information away from its true or accurate position as the result of systematic error.

Binder – Asphalt cement or modified asphalt cement that binds the aggregate particles into a dense mass.

Boulders – Rock fragment, often rounded, with an average dimension larger than 300 mm (12 in.).

Bulk Density – The mass per volume of a material, including any voids that may occur within the volume.

Bulk specific gravity – The ratio of the mass, in air, of a volume of aggregate or compacted asphalt concrete mix (including the permeable and impermeable voids in the particles, but not including the voids between particles) to the mass of an equal volume of water.

Bulk specific gravity (SSD) – The ratio of the mass, in air, of a volume of aggregate or compacted asphalt concrete mix, including the mass of water within the voids (but not including the voids between particles), to the mass of an equal volume of water. (See saturated surface dry.)

Calibration – A process that establishes the relationship (traceability) between the results of a measurement instrument, measurement system, or a material measure and the corresponding values assigned to a reference standard.

Check – A specific type of inspection and/or measurement performed on equipment and materials to indicate compliance or otherwise with stated criteria.

Clay – Fine-grained soil that exhibits plasticity over a range of water contents, and that exhibits considerable strength when dry. Also, that portion of the soil finer than 2 µm.

Cobble – Rock fragment, often rounded, with an average dimension between 75 and 300 mm (3 and 12 in.).

Cohesionless soil – Soil with little or no strength when dry and unconfined or when submerged, such as sand.

Cohesive soil – Soil with considerable strength when dry and that has significant cohesion when unconfined or submerged.

Compaction – Densification of a soil or asphalt concrete pavement by mechanical means.

Compaction curve (Proctor curve or moisture-density curve) – The curve showing the relationship between the dry unit weight or density and the water content of a soil for a given compactive effort.

Compaction test (moisture-density test) – Laboratory compaction procedure in which a soil of known water content is placed in a specified manner into a mold of given dimensions, subjected to a compactive effort of controlled magnitude, and the resulting density determined.

Compressibility – Property of a soil or rock relating to susceptibility to decrease in volume when subject to load.

Consolidation – In the placement of portland cement concrete (PCC) it is the removal of entrapped air by either tamping or vibrating the material.

Constructor – The builder of a project. The individual or entity responsible for performing and completing the construction of a project required by the contract documents. Often called a contractor, since this individual or entity contracts with the owner.

Crusher-run – The total unscreened product of a stone crusher.

Delivery tolerances – Permissible variations from the desired proportions of aggregate and asphalt cement delivered to the pug mill.

Density – The ratio of mass to volume of a substance. Usually expressed in kg/m^3 (lb/ft^3).

Design professional – The designer of a project. This individual or entity may provide services relating to the planning, design, and construction of a project, possibly including materials testing and construction inspection. Sometimes called a “contractor”, since this individual or entity contracts with the owner.

Dryer – An apparatus that dries aggregate and heats it to specified temperatures.

Dry mix time – The time interval between introduction of aggregate into the pug mill and the addition of asphalt cement.

Durability – The property of concrete that describes its ability to resist disintegration by weathering and traffic. Included under weathering are changes in the pavement and aggregate due to the action of water, including freezing and thawing.

Effective diameter (effective size) – D_{10} , particle diameter corresponding to 10 percent finer or passing.

Embankment – Controlled, compacted material between the subgrade and subbase or base in a roadway.

Field Operating Procedure (FOP) – Procedure used in field testing on a construction site or in a field laboratory. (Based on AASHTO, ASTM or WAQTC test methods.)

Fineness modulus – A factor equal to the sum of the cumulative percentages of aggregate retained on certain sieves divided by 100; the sieves are 150 mm (6”), 75 mm (3”), 37.5 mm (1 ½”), 19.0 mm (¾”), 9.5 mm (3/8”), 4.75 mm (No. 4), 2.36 mm (No. 8), 1.18 mm (No. 16), 0.60 mm (No. 30), 0.30 mm (No. 50), and 0.15 mm (No. 100). Used in the design of concrete mixes. The lower the fineness modulus, the more water/cement paste that is needed to coat the aggregate.

Fines – Portion of a soil or aggregate finer than a 75 μm (No. 200) sieve. Also silts and clays.

Free water – Water on aggregate available for reaction with hydraulic cement. Mathematically, the difference between total moisture content and absorbed moisture content.

Glacial till – Material deposited by glaciation, usually composed of a wide range of particle sizes, which has not been subjected to the sorting action of water.

Gradation (grain-size or particle-size distribution) – The proportions by mass of a soil or fragmented rock distributed by particle size.

Gradation analysis (grain size analysis, particle-size or sieve analysis) – The process of determining grain-size distribution by separation of sieves with different size openings.

Hot aggregate storage bins – Bins that store heated and separated aggregate prior to final proportioning into the mixer.

Hot mix asphalt (HMA) – High quality, thoroughly controlled hot mixture of asphalt cement and well-graded, high quality aggregate. The term Warm Mix Asphalt (WMA) is interchangeable with Hot Mix Asphalt (HMA) in this Manual. See WMA for more information.

Hydraulic cement – Cement that sets and hardens by chemical reaction with water.

Independent assurance (IA)—Activities that are an unbiased and independent evaluation of all the sampling and testing (or inspection) procedures used in the quality assurance program. [IA provides an independent verification of the reliability of the acceptance (or verification) data obtained by the. The results of IA testing or inspection are not to be used as a basis of acceptance. IA provides information for quality system management.]

In situ – Rock or soil in its natural formation or deposit.

Liquid limit – Water content corresponding to the boundary between the liquid and plastic states.

Loam – A mixture of sand, silt and/or clay with organic matter.

Lot – A quantity of material to be controlled. It may represent a specified mass, a specified number of truckloads, a linear quantity, or a specified time period during production.

Manual proportioning control – A control system in which proportions of the aggregate and asphalt fractions are controlled by means of gates or valves that are opened and closed by manual means. The system may or may not include power assisted devices in the actuation of gate and valve opening and closing.

Materials and methods specifications – Also called prescriptive specifications. Specifications that direct the Constructor (Contractor) to use specified materials in definite proportions and specific types of equipment and methods to place the material.

Maximum size – One sieve larger than nominal maximum size.

Maximum particle size – First sieve to retain any material.

Mesh – The square opening of a sieve.

Moisture content (Soils and Aggregate)– The ratio, expressed as a percentage, of the mass of water in a material to the dry mass of the material.

Moisture content (Asphalt)– The ratio, expressed as a percentage, of the mass of water in a material to the wet mass of the material.

Nominal maximum size – One sieve larger than the first sieve to retain more than 10 percent of the material using an agency specified set of sieves based on cumulative percent retained. Where large gaps between specification sieves exist, intermediate sieve(s) may be inserted to determine nominal maximum size.

Nuclear gauge – Instruments used to measure in-place density, moisture content, or asphalt content through the measurement of nuclear emissions.

Optimum moisture content (optimum water content) – The water content at which a soil can be compacted to a maximum dry density by a given compactive effort.

Organic soil – Soil with a high organic content.

Paste – Mix of water and hydraulic cement that binds aggregate in portland cement concrete (PCC).

Penetration – The consistency of a bituminous material, expressed as the distance in tenths of a millimeter (0.1 mm) that a standard needle vertically penetrates a sample of the material under specified conditions of loading, time, and temperature.

Percent compaction – The ratio of density of a soil, aggregate, or asphalt concrete mix in the field to maximum density determined by a standard compaction test, expressed as a percentage.

Plant screens – Screens located between the dryer and hot aggregate storage bins that separate the heated aggregates by size.

Plastic limit – Water content corresponding to the boundary between the plastic and the semisolid states.

Plasticity – Property of a material to continue to deform indefinitely while sustaining a constant stress.

Plasticity index – Numerical difference between the liquid limit and the plastic limit and, thus, the range of water content over which the soil is plastic.

Portland cement – Hydraulic cement produced by pulverizing portland cement clinker.

Portland cement concrete (PCC) – A controlled mix of aggregate, portland cement, and water, and possibly other admixtures.

PCC batch plant – A manufacturing facility for producing portland cement concrete.

Process control – See Quality control.

Proficiency samples – Homogeneous samples that are distributed and tested by two or more laboratories. The test results are compared to assure that the laboratories are obtaining the same results.

Pugmill – A shaft mixer designed to mix aggregate and cement.

Quality assurance (QA)—(1) All those planned and systematic actions necessary to provide confidence that a product or facility will perform satisfactorily in service; or (2) making sure the quality of a product is what it should be. [QA addresses the overall process of obtaining the quality of a service, product, or facility in the most efficient, economical, and satisfactory manner possible. Within this broad context, QA includes the elements of quality control, independent assurance, acceptance, dispute resolution etc. The use of the term QA/QC or QC/QA is discouraged and the term QA should be used. QA involves continued evaluation of the activities of planning, design, development of plans and specifications, advertising and awarding of contracts, construction, and maintenance, and the interactions of these activities.]

Quality assurance specifications—Specifications that require contractor quality control and agency acceptance activities throughout production and placement of a product. Final acceptance of the product is usually based on a statistical sampling of the measured quality level for key quality characteristics. [QA specifications typically are statistically based specifications that use methods such as random sampling and lot-by-lot testing, which let the contractor know if the operations are producing an acceptable product.]

Quality control (QC) - also called *process control*. The system used by a contractor to monitor, assess and adjust their production or placement processes to ensure that the final product will meet the specified level of quality. Quality control includes sampling, testing, inspection and corrective action (where required) to maintain continuous control of a production or placement process.

Reclaimed Asphalt Pavement (RAP) - is the term given to removed and/or reprocessed pavement materials containing asphalt and aggregates. These materials are typically generated when asphalt pavements are removed either by milling or full-depth removal. When properly crushed and screened, RAP consists of high-quality, well-graded aggregates coated by asphalt cement that may be recycled as a portion of new asphalt pavement.

Random sampling – Procedure for obtaining non-biased, representative samples.

Sand – Particles of rock passing the 4.75 mm (No. 4) sieve and retained on the 75 μ m (No. 200) sieve.

Saturated surface dry (SSD) – Condition of an aggregate particle, asphalt concrete pavement or portland cement concrete (PCC) core, or other porous solid when the permeable voids are filled with water, but no water is present on exposed surfaces. (See bulk specific gravity.)

Segregation – The separation of aggregate by size resulting in a non-uniform material.

SHRP – The Strategic Highway Research Program (SHRP) established in 1987 as a five-year research program to improve the performance and durability of roads and to make those roads safe for both motorists and highway workers. SHRP research funds were partly used for the development of performance-based specifications to directly relate laboratory analysis with field performance.

Sieve – Laboratory apparatus consisting of wire mesh with square openings, usually in circular or rectangular frames.

Silt – Material passing the 75 μ m (No. 200) sieve that is non-plastic or very slightly plastic, and that exhibits little or no strength when dry and unconfined. Also, that portion of the soil finer than 75 μ m and coarser than 2 μ m.

Slump – Measurement related to the workability of concrete.

Soil – Natural occurring sediments or unconsolidated accumulations of solid particles produced by the physical and chemical disintegration of rocks, and which may or may not contain organic matter.

Specific gravity – The ratio of the mass, in air, of a volume of a material to the mass of an equal volume of water.

Stability – The ability of an asphalt concrete to resist deformation from imposed loads. Stability is dependent upon internal friction, cohesion, temperature, and rate of loading.

Standardization—A process that determines (1) the correction or correction factor to be applied to the result of a measuring instrument, measuring system, material measure or reference material when its values are compared to the values realized by standards, (2) the adjustment to be applied to a piece of equipment when its performance is compared with that of an accepted standard or process.

Stratified random sampling – Procedure for obtaining non-biased, representative samples in which the established lot size is divided into equally-sized sublots.

Subbase – A layer of selected material constructed between the subgrade and the base course in a flexible asphalt concrete pavement roadway, or between the subgrade and Portland Cement Concrete (PCC) pavement in a rigid PCC roadway.

Subgrade – Natural soil prepared and compacted to support a structure or roadway pavement.

Sublot – A segment of a lot chosen to represent the total lot.

Superpave™ – Superpave™ (Superior Performing Asphalt Pavement) is a trademark of the Strategic Highway Research Program (SHRP). Superpave™ is a product of the SHRP asphalt research. The Superpave™ system incorporates performance-based asphalt materials characterization with design environmental conditions to improve performance by controlling rutting, low temperature cracking and fatigue cracking. The three major components of Superpave™ are the asphalt binder specification, the mix design and analysis system, and a computer software system.

Theoretical maximum specific gravity – The ratio of the mass of a given volume of asphalt concrete with no air voids to the mass of an equal volume of water, both at a stated temperature commonly referred to as the “Rice” value.

Topsoil – Surface soil, usually containing organic matter.

Traceability—The property of a result of a measurement whereby it can be related to stated references, usually national or international standards, through an unbroken chain of comparisons all having stated uncertainties.

Uncertainty—A parameter associated with the result of a measurement that defines the range of the values that could be attributed to the measured quantity.

Uniformity coefficient – C_u , a value employed to quantify how uniform or well-graded an aggregate is: $C_u = D_{60}/D_{10}$. 60 percent of the aggregate, by mass, has a diameter smaller than D_{60} and 10 percent of the aggregate, by mass, has a diameter smaller than D_{10} .

Unit weight – The ratio of weight to volume of a substance. The term “density” is more commonly used.

μm – Micro millimeter (micron) used as measurement for sieve size.

Verification of calibration - A process that establishes whether the results of a previously calibrated measurement instrument, measurement system, or material measure are stable.

Verification sampling and testing—See acceptance sampling and testing.

Viscosity – A measure of the resistance to flow; one method of measuring the consistency of asphalt.

- **Absolute viscosity** – A method of measuring viscosity using the “poise” as the basic measurement unit. This method is used at a temperature of 60°C, typical of hot pavement.
- **Kinematic viscosity** – A method of measuring viscosity using the stoke as the basic measurement unit. This method is used at a temperature of 135°C, typical of hot asphalt at a plant.

Void in the mineral aggregate (VMA) – The volume of inter-granular void space between aggregate particles of compacted asphalt concrete pavement that includes air and asphalt; expressed as a percentage of the bulk volume of the compacted paving mixture.

Voids filled with asphalt – The portion of the void in the mineral aggregate (VMA) that contains asphalt; expressed as a percentage of the bulk volume of mix or the VMA.

Warm Mix Asphalt (WMA) - The generic term for a variety of technologies that allow the producers of HMA pavement material to lower the temperatures at which the material is mixed and placed on the road. Reductions from HMA temperatures of 50 to 100 degrees Fahrenheit are documented. Three general technologies are used at this time to decrease the mix and compaction temperatures including: chemical additives, organic additives

(waxes) and foaming with water. Sampling and testing of WMA is done the same as with HMA so these terms are interchangeable in this Manual.

Wet mixing period – The time interval between the beginning of application of asphalt material and the opening of the mixer gate.

Zero air voids curve (saturation curve) – Curve showing the zero air voids density as a function of water content. Points that define the curve are calculated in accordance with the addendum of WAQTC FOP for AASHTO T 99/ T 180.

Calibration of Mechanical Compaction Hammer/Rammer SP 2

1. Scope

This practice sets forth the apparatus, procedures, and materials necessary to calibrate a mechanical compaction hammer used in ATM 417, WAQTC FOP for AASHTO T 99/T 180, AASHTO T 245; and ASTM D 698/D 1557 in accordance with ASTM E 2168.

This test method involves potentially hazardous materials, operations and equipment. This method does not purport to address all of the safety problems associated with its use.

2. Apparatus

- Hand-operated compaction hammer and compaction pedestal conforming to the requirements of WAQTC FOP for AASHTO T 99/T 180, AASHTO T 245; and ASTM D 698/D 1557.
- Mechanical compaction hammer and pedestal conforming to the requirements of ATM 417, WAQTC FOP for AASHTO T 99/T 180, AASHTO T 245, and ASTM D 698/D 1557.
- Marshall and Proctor compaction molds, bases, collars and rubber plugs (roughly 50 mm (2") thick and cut to fit bottom of mold).
- Caliper capable of measuring 25 mm to an accuracy of 0.01 mm.
- Lead deformation apparatus, consisting of an anvil, guide collar and striking pin.
- Lead test cylinders having a maximum weight spread of 0.06 grams between the heaviest and the lightest cylinder, a length of 17.2 ± 0.1 mm and a diameter of 7.87 ± 0.05 mm. A minimum of ten test cylinders are required for the calibration of one compaction hammer (However as many as 100 test cylinders may be required.)

Note 1: Calibration Kit CN-4242 and Lead Cylinders CN-4245 available from Soil Test have been found satisfactory.

3. Procedure--General

1. Inspect and adjust the mechanical and hand-operated compaction hammers to conform to the requirements of ATM T 417, WAQTC FOP for AASHTO T 99, T 180, AASHTO T 245; and ASTM D 698 & D 1557.
2. Select a set of lead cylinders from the same lot or shipment. Remove any burrs from the ends of the cylinders using a fine grade of emery cloth.

Note 2: Deformation of the test cylinders is affected by changes in temperature. Take precautions to maintain the temperature of the test cylinders within 3°C of the temperature of the mechanical and hand-operated compaction hammers during the calibration procedure. All testing may be done at room temperature.

3. Measure and record, to the nearest 0.01 mm, the original length of the test cylinders.

4. Procedure—Hand Operated Manual Hammer

1. Place the compaction mold base plate on the compaction pedestal.
2. Assemble the deformation apparatus and place on the base plate.
3. Gently place a compaction mold with collar on the base plate.

4. Gently place the hand-operated hammer on top of the striking pin and, with the guide shaft held vertical; apply one drop of the hammer.
5. Measure and record, to the nearest 0.01 mm, the final length of the test cylinder.
6. Using new test cylinders each time, repeat steps 2 through 5 until five (5) deformation values are obtained that do not vary by more than ± 2.0 percent from the average value of all values within this range.

5. Procedure—Mechanically Operated Hammer

1. Assemble a compaction base, mold and collar. Place a rubber plug in the mold assembly and operate the compaction hammer for a minimum of 25 drops to allow friction in the parts to become constant. Remove the rubber plug.
2. Place the compaction mold base plate on the compaction pedestal.
3. Assemble the deformation apparatus and place on the base plate.
4. Gently place a compaction mold with collar on the base plate.
5. Gently place the mechanical hammer on top of the striking pin and, with the guide shaft held vertical; apply one drop of the hammer.
6. The mechanical compaction hammer shall operate automatically using the same technique that would be used in the actual test method. Raising and releasing the hammer manually or by any other procedure is not allowed.
7. Measure and record, to the nearest 0.01 mm, the final length of the test cylinder.
8. Using new test cylinders each time, repeat steps 3 through 7 until five (5) deformation values are obtained that do not vary by more than ± 2.0 percent from the average value of all values within this range.

6. Calibration Comparison and Adjustment

1. Calculate the percentage difference between the average deformation values of the mechanical and hand-operated compaction hammers. If the difference is less than or equal to 2.0 percent the mechanical compaction hammer is ready for use.
2. If the difference is greater than 2.0 percent, adjust the weight of the mechanical hammer and repeat steps 3 through 7 of the Mechanically Operated Hammer Procedure, until the mean value of 3 sets of data is equal to, or less than 2.0 percent.

7. Report

1. All compaction hammers shall be calibrated every 12 months or prior to use if the existing calibration is more than one (1) year old.
2. The original calibration certificate and test data shall be filed at the calibrating laboratory.
3. A copy of the calibration certificate shall be kept with the Compaction Hammer.

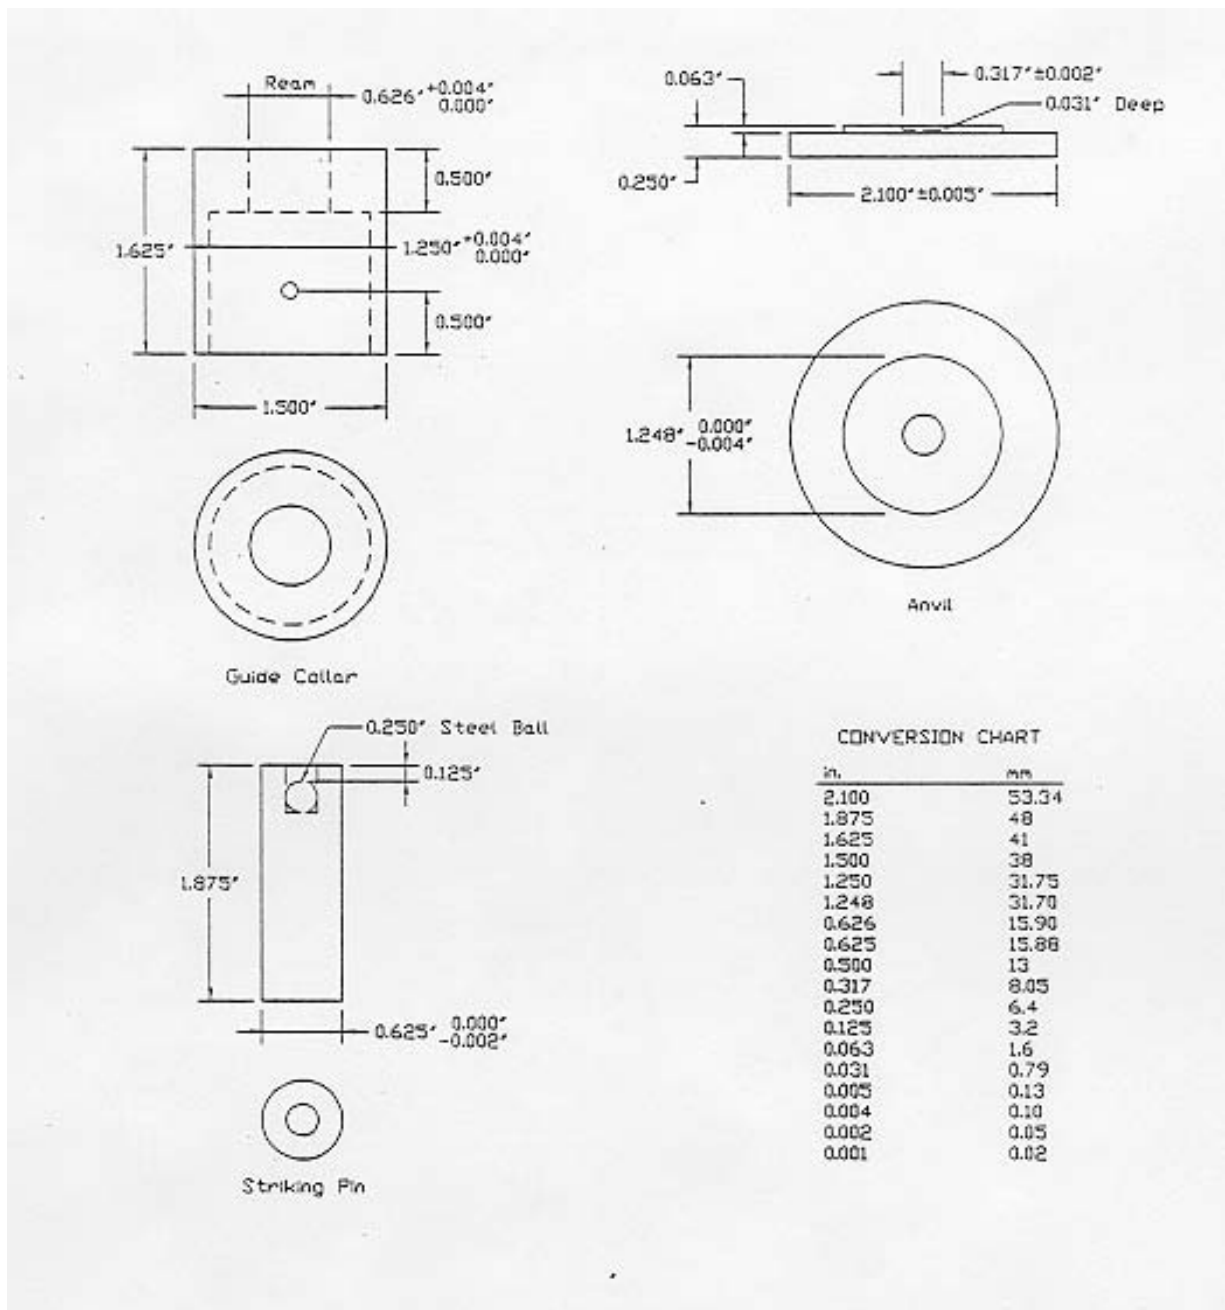


Figure 1.
LEAD DEFORMATION APPARATUS

This page intentionally left blank.

Random Sampling SP 4

1. Significance

Sampling and testing are two of the most important functions in quality acceptance /quality control (QA/QC). Data from the tests are the tools with which the quality of product is controlled. For this reason, great care must be used in following standardized sampling and testing procedures. This practice is useful for determining the location or time, or both, to take a sample in order to minimize any unintentional bias on the part of the person taking the sample.

The selection procedures and examples in this standard provide a practical approach for ensuring that construction material samples are obtained in a random manner. Additional details concerning the number of sample increments, the number of samples, the quantities of material in each, and the procedures for extracting sample increments or samples from the construction lot or process are contained in the Construction Manual and the individual test procedures. This standard contains examples using road and paving materials. The concepts outlined here are applicable to the random sampling of any construction material.

2. Scope


The procedure presented here eliminates bias in sampling materials when followed carefully. Randomly selecting a set of numbers from a table or calculator will eliminate the possibility for bias. Random numbers are used to identify sampling times and/or locations within a lot or subplot. This method does not cover how to sample, but rather how to determine sampling times and/or locations.

3. Sampling Concepts

A lot is the quantity of material evaluated by QA/QC procedures. A lot is a preselected quantity that may represent hours of production, a quantity or number of loads of material, or an interval of time. A lot may be comprised of several portions that are called sublots or units. The number of sublots comprising a lot will be determined by the agency's specifications

Stratified Random Sampling: Stratified random sampling divides the lot into a specified number of sublots or units and then determines each sample location within a distinct subplot.

All random sampling shall be stratified random sampling unless otherwise directed.

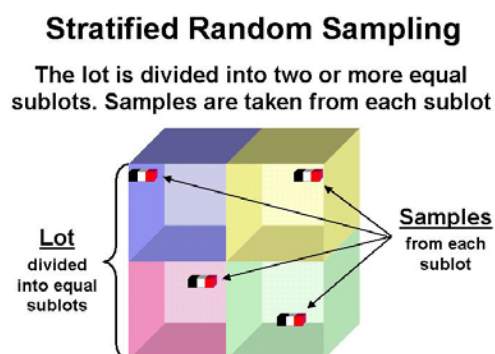

4. Instructions for Using the Three-Digit Table of Random Numbers

Table 1 consists of 1,000 numbers from 0.000 to 0.999. Each number appears only once in the Table of 100 rows by 10 columns. The Table is most effectively used when a row and column are randomly selected and the entered value from the Table is then used for sample selection. Several methods of selection of row and column are available including:

1. Use of the RANDOM function in pocket calculators (if available) to select row and column. For example, for selection of row: the RANDOM function generates 0.6202. Then the row to be used is $0.620 \times \text{the number of rows} = 0.620(100) = 62.0$ or 62. Likewise for the column, the RANDOM function generates 0.958 and the column is $0.958(10) = 9.58$ or 10. The random number to be used for the sample is in row 62, column 10 = 0.460.
2. Similarly, if Microsoft Excel is available, the RAND function can be used to generate random numbers for selection of row and column. This can be accomplished by selecting an open cell in Excel entering: =RAND() or: =rand(). Do this once for a row and a second for column, multiplying as explained above.
3. The first two or last two digits in the next automobile license plate you see. Put a decimal in front of these numbers and use this to compute Row/Column numbers as described in section 4(1).
4. Start a digital stop watch and stop it several seconds later, using the decimal part of the seconds as multipliers to determine your Row/Column number(s).

Table 1

Row\Column	1	2	3	4	5	6	7	8	9	10
1	0.910	0.921	0.889	0.985	0.697	0.562	0.701	0.284	0.534	0.519
2	0.769	0.814	0.210	0.758	0.846	0.113	0.312	0.716	0.975	0.729
3	0.722	0.220	0.726	0.942	0.825	0.177	0.120	0.558	0.979	0.451
4	0.872	0.772	0.338	0.374	0.000	0.387	0.491	0.647	0.445	0.053
5	0.850	0.836	0.145	0.216	0.270	0.109	0.590	0.882	0.740	0.434
6	0.291	0.780	0.782	0.306	0.470	0.712	0.252	0.630	0.231	0.694
7	0.295	0.502	0.615	0.541	0.765	0.092	0.376	0.523	0.551	0.733
8	0.761	0.370	0.278	0.288	0.256	0.352	0.064	0.195	0.334	0.652
9	0.790	0.750	0.402	0.182	0.577	0.391	0.214	0.481	0.680	0.348
10	0.547	0.011	0.355	0.587	0.359	0.310	0.192	0.545	0.487	0.925
11	0.868	0.049	0.505	0.139	0.705	0.007	0.633	0.754	0.124	0.280
12	0.384	0.968	0.483	0.203	0.513	0.583	0.637	0.477	0.957	0.515
13	0.996	0.665	0.658	0.412	0.149	0.673	0.103	0.344	0.619	0.263
14	0.804	0.242	0.662	0.135	0.248	0.173	0.398	0.459	0.744	0.156
15	0.440	0.331	0.128	0.737	0.529	0.313	0.683	0.839	0.636	0.245
16	0.042	0.027	0.337	0.142	0.196	0.036	0.516	0.074	0.666	0.277
17	0.497	0.903	0.444	0.822	0.886	0.230	0.463	0.234	0.185	0.068
18	0.508	0.999	0.469	0.480	0.448	0.544	0.121	0.260	0.843	0.078
19	0.672	0.871	0.540	0.025	0.548	0.978	0.495	0.138	0.202	0.281
20	0.031	0.059	0.241	0.431	0.897	0.198	0.559	0.946	0.206	0.003
21	0.775	0.668	0.441	0.993	0.644	0.634	0.591	0.604	0.341	0.865

22	0.174	0.100	0.324	0.651	0.935	0.110	0.292	0.747	0.213	0.249
23	0.465	0.309	0.961	0.006	0.401	0.950	0.038	0.305	0.907	0.166
24	0.369	0.046	0.484	0.170	0.377	0.416	0.640	0.967	0.399	0.608
25	0.597	0.864	0.063	0.725	0.146	0.687	0.330	0.394	0.693	0.928
26	0.052	0.629	0.351	0.586	0.896	0.020	0.860	0.490	0.881	0.913
27	0.892	0.922	0.360	0.253	0.127	0.067	0.189	0.815	0.084	0.018
28	0.832	0.159	0.178	0.618	0.800	0.255	0.890	0.456	0.757	0.383
29	0.095	0.349	0.157	0.426	0.554	0.992	0.413	0.885	0.924	0.148
30	0.778	0.981	0.237	0.906	0.703	0.970	0.874	0.810	0.949	0.472
31	0.917	0.767	0.002	0.714	0.899	0.867	0.824	0.326	0.621	0.561
32	0.760	0.593	0.589	0.696	0.835	0.600	0.856	0.682	0.415	0.518
33	0.180	0.625	0.550	0.447	0.817	0.689	0.614	0.582	0.678	0.646
34	0.301	0.532	0.329	0.500	0.436	0.575	0.536	0.564	0.671	0.372
35	0.397	0.258	0.653	0.290	0.557	0.418	0.358	0.386	0.888	0.322
36	0.080	0.347	0.244	0.251	0.176	0.187	0.443	0.212	0.315	0.977
37	0.379	0.155	0.411	0.507	0.009	0.041	0.308	0.169	0.137	0.066
38	0.062	0.201	0.831	0.297	0.098	0.998	0.265	0.105	0.094	0.927
39	0.863	0.884	0.916	0.183	0.895	0.130	0.948	0.087	0.920	0.215
40	0.717	0.781	0.984	0.037	0.909	0.706	0.973	0.304	0.877	0.802
41	0.635	0.667	0.934	0.795	0.763	0.592	0.158	0.699	0.838	0.656
42	0.624	0.891	0.731	0.806	0.692	0.617	0.585	0.681	0.980	0.649
43	0.012	0.660	0.457	0.482	0.724	0.553	0.745	0.820	0.503	0.439
44	0.364	0.546	0.514	0.343	0.571	0.407	0.610	0.866	0.336	0.535
45	0.400	0.720	0.261	0.293	0.560	0.421	0.389	0.425	0.218	0.325
46	0.179	0.446	0.279	0.318	0.777	0.243	0.211	0.307	0.222	0.275
47	0.133	0.140	0.969	0.076	0.033	0.631	0.236	0.161	0.396	0.129
48	0.311	0.172	0.663	0.752	0.930	0.154	0.122	0.197	0.485	0.983
49	0.015	0.250	0.517	0.951	0.090	0.855	0.165	0.880	0.805	0.816
50	0.869	0.837	0.848	0.741	0.773	0.008	0.784	0.040	0.912	0.709
51	0.926	0.627	0.958	0.894	0.734	0.723	0.638	0.670	0.937	0.798
52	0.314	0.791	0.047	0.727	0.556	0.823	0.282	0.620	0.588	0.492
53	0.378	0.645	0.136	0.403	0.474	0.346	0.410	0.613	0.435	0.264
54	0.257	0.531	0.499	0.150	0.385	0.289	0.086	0.111	0.353	0.079
55	0.698	0.004	0.175	0.143	0.972	0.997	0.029	0.061	0.965	0.093
56	0.940	0.730	0.794	0.762	0.826	0.858	0.648	0.616	0.787	0.584
57	0.829	0.900	0.953	0.793	0.274	0.566	0.423	0.117	0.809	0.254
58	0.466	0.989	0.419	0.395	0.936	0.579	0.914	0.643	0.286	0.083
59	0.299	0.224	0.449	0.776	0.060	0.473	0.235	0.417	0.898	0.097
60	0.227	0.238	0.205	0.302	0.748	0.878	0.017	0.601	0.186	0.987
61	0.085	0.131	0.526	0.075	0.163	0.430	0.363	0.032	0.104	0.019
62	0.039	0.537	0.043	0.259	0.141	0.494	0.171	0.609	0.428	0.460
63	0.188	0.088	0.654	0.690	0.316	0.438	0.808	0.964	0.193	0.549
64	0.167	0.152	0.462	0.267	0.320	0.160	0.641	0.199	0.677	0.901

65	0.342	0.096	0.099	0.622	0.786	0.028	0.569	0.947	0.755	0.990
66	0.611	0.818	0.932	0.857	0.081	0.408	0.427	0.840	0.207	0.168
67	0.077	0.686	0.594	0.605	0.573	0.669	0.380	0.246	0.908	0.876
68	0.107	0.801	0.718	0.498	0.893	0.707	0.530	0.797	0.453	0.350
69	0.598	0.327	0.406	0.904	0.675	0.626	0.509	0.861	0.382	0.414
70	0.184	0.366	0.555	0.455	0.021	0.323	0.684	0.071	0.268	0.108
71	0.153	0.164	0.132	0.228	0.939	0.070	0.209	0.527	0.887	0.919
72	0.057	0.452	0.266	0.089	0.356	0.217	0.971	0.974	0.051	0.574
73	0.420	0.807	0.732	0.303	0.715	0.743	0.014	0.580	0.873	0.830
74	0.388	0.512	0.833	0.982	0.676	0.373	0.768	0.405	0.659	0.862
75	0.779	0.501	0.736	0.679	0.538	0.010	0.273	0.335	0.581	0.371
76	0.612	0.796	0.764	0.572	0.437	0.576	0.409	0.704	0.467	0.232
77	0.294	0.271	0.811	0.602	0.700	0.995	0.433	0.854	0.239	0.933
78	0.875	0.262	0.367	0.929	0.102	0.623	0.476	0.711	0.819	0.915
79	0.655	0.181	0.345	0.506	0.106	0.570	0.918	0.134	0.528	0.496
80	0.963	0.285	0.650	0.024	0.317	0.520	0.565	0.960	0.542	0.147
81	0.050	0.223	0.986	0.522	0.125	0.751	0.988	0.956	0.300	0.001
82	0.114	0.783	0.533	0.056	0.221	0.381	0.789	0.287	0.058	0.026
83	0.911	0.392	0.847	0.849	0.319	0.298	0.943	0.362	0.944	0.606
84	0.828	0.719	0.954	0.708	0.552	0.458	0.424	0.853	0.905	0.691
85	0.116	0.821	0.191	0.082	0.879	0.488	0.661	0.035	0.595	0.702
86	0.739	0.938	0.045	0.746	0.013	0.504	0.842	0.735	0.759	0.442
87	0.728	0.803	0.771	0.091	0.632	0.664	0.931	0.792	0.225	0.328
88	0.753	0.710	0.475	0.945	0.785	0.657	0.454	0.721	0.118	0.200
89	0.486	0.543	0.034	0.511	0.340	0.404	0.799	0.607	0.883	0.022
90	0.639	0.479	0.269	0.468	0.354	0.365	0.333	0.429	0.464	0.229
91	0.461	0.226	0.123	0.390	0.525	0.493	0.568	0.283	0.115	0.044
92	0.422	0.240	0.208	0.219	0.272	0.112	0.742	0.144	0.065	0.204
93	0.966	0.073	0.030	0.233	0.361	0.596	0.126	0.276	0.994	0.962
94	0.151	0.119	0.194	0.450	0.991	0.959	0.055	0.023	0.072	0.841
95	0.852	0.685	0.162	0.774	0.845	0.738	0.770	0.005	0.339	0.976
96	0.813	0.952	0.069	0.539	0.941	0.048	0.749	0.016	0.766	0.695
97	0.603	0.859	0.628	0.902	0.870	0.827	0.393	0.923	0.812	0.524
98	0.489	0.510	0.521	0.756	0.713	0.478	0.788	0.247	0.296	0.563
99	0.578	0.101	0.567	0.674	0.834	0.375	0.642	0.471	0.321	0.844
00	0.332	0.599	0.955	0.688	0.190	0.357	0.368	0.432	0.054	0.851

5. Random Number Sampling Procedures

Determine the number of random numbers necessary for each sample location from Table 2.

Table 2

Sample Type/ Method	# of Random Numbers Required
Oil from plant or truck	1
T 2/T 168 from Belt	1
T 2/T 168 from Truck	1
T 2/T 168 from Roadway	2
T 2/T 168 from Windrow	1
TM 11 Core	2
TM 2 Plastic Concrete	1
TM 12 Grout	1

Multiply the random number by the unit quantity in each subplot to determine sample location. When a sample is taken from a discrete location such as a truck load, and the sample method treats the load as a unit, sample per the procedure from the truck that contains the determined location.

Sample locations are for that sample only and are not reused for other samples. This would apply for samples of in place soil, aggregate, hot mix asphalt or cores. Each would require a separate set of random numbers. When two random numbers are used, such as in hot mix asphalt, the first random number would be multiplied by the length to determine where the sample would be taken along the project. The second would be multiplied by the width to determine where, widthwise, the sample would be taken. When the random number identified location falls within the beginning, end or edge, adjust the location to comply with the sampling method requirements.

Two random numbers Example:

Given: Sublot length = 3,340 feet

Sublot width = 12 feet

Random numbers for Row = 0.0262 and 0.3687

Random numbers for Column = 0.1696 and 0.3410

Find: length and width locations of sample

Solution: First Row number is: $10(0.0262) = 0.262$ or Row 1

First Column number is: $100(0.1696) = 16.96$ or Column 17

From Table 1, Row 1, Column 17, the random number for Length is: 0.497

So the sample location for length is: $0.497(3,340') = 1,659.98$ or 1,660' from beginning

If sampling material requiring only 1 random number this sample is located.

Second Row number is: $10(0.3687) = 3.687$ or Row 4

Second Column number is: $100(0.3410) = 34.1$ or Column 34

From Table 1, Row 4, Column 34, the random number for width is: 0.500

So the sample location for width is: $12(0.500) = 6'$ from the left edge of the subplot

When developing a sampling plan, determine a new set of random numbers for each sample required. For example, if the testing frequency specified indicates there will be twenty samples from a material, determine twenty different random number identified locations for the plan.

Additional examples are available in the Random Number section of all WAQTC modules as well as in ASTM D 3665.

Rounding and Precision in Materials Test Reporting SP 6

1. Scope

This standard practice provides a procedure for rounding off numbers generated during the process of calculating materials testing results when a specific test method does not specify rounding procedures.

2. Calculation Procedures

- 2.1 All test results should be reported to a significant, practical, and accurate value. This can be achieved using the following procedures:
- 2.2 If the first digit to the right of the place to which the calculation is to be reported ends in 0, 1, 2, 3, or 4, the value of that place is not changed. If the rounded number ends in 0, the 0 should be written down. For example, if the result of a calculation is to be rounded to the tenth then 5.6489 rounds to 5.6.
- 2.3 If the first digit to the right of the place to which the calculation is to be reported ends in 5, 6, 7, 8, or 9, the value of that place is increased by one. For example, if the result of a calculation is to be rounded to the tenth, then 5.6543 rounds to 5.7; 7.9722 rounds to 8.0; 0.054 rounds to 0.1.
- 2.4 Intermediate calculations are carried out to one more decimal place than that required in the final result. For example, where the final answer is to be reported to the whole percent, intermediate calculations will be carried out to the tenth of a percent (0.1%).
- 2.5 Most calculators carry 8 digits internally regardless of how many digits are shown in the display. When it is directed to round to a certain level of precision, this means round that value immediately. If the calculator shows a result as 7.45, it may be carrying 7.44537901. If the directions call for this intermediate result to be given to the hundredth, the calculator must be cleared and 7.45 entered. This rounded value must be entered in the calculator in order to remove unusable figures. As another example, if the value 3.4675489 results from a calculation and the directions are to round that result to the tenth, then the calculator must be cleared and the value 3.5 entered.

This page intentionally left blank.

Determination of Outlier Test Results SP 7

1. Scope

This standard practice provides a mechanism for rejecting individual test values that may misrepresent the physical properties of a material lot. The method statistically identifies a non-representative "outlier" and justifies its removal from the remaining test data for the lot.

2. General

1. When a test result is clearly a result of a gross deviation from prescribed sampling or testing procedure, the test result should be discarded, without further analysis. When no direct evidence of sampling and/or testing errors exists, the lot data will be statistically evaluated for the presence of an outlier.
2. An outlying test result will be assumed to be non-characteristic of the overall quality of the material tested. Outlying test results will be excluded from the price adjustment calculation, by either documental evidence or through statistical analysis.

3. Basis of Statistical Criteria For Outliers

All test results in a lot are included in the calculation of the numerical value of a sample criterion (or statistic), which is then compared with a critical value based on the theory of random sampling from a normal distribution to determine whether the doubtful test result is to be retained or rejected. The critical value is that value of the sample criterion that would be exceeded by chance with 5% total probability. This 5% probability is the risk of erroneously rejecting a good observation and is the Department's defined outlier threshold limit.

4. Procedure

- 4.1 Calculate the arithmetic mean \bar{x} of all test results for the lot using the following formula:

$$\bar{x} = \frac{\sum X}{n}$$

Where: \sum = summation of
 X = individual test value to x_n
 n = total number of test values

And where: \bar{x} is rounded to the nearest 0.1 percent for density and all sieve sizes except the 0.075 mm (No. 200) sieve.

\bar{x} is rounded to the nearest 0.01 percent for asphalt content and the 0.075 mm (No. 200) sieve.

- 4.2 Calculate sample standard deviation (s) of all test results for the lot using the following formula:

$$s = \sqrt{\frac{n \sum (x^2) - (\sum x)^2}{n(n-1)}}$$

Where: s = standard deviation of the lot
 $\sum(x^2)$ = summation of the squares of individual test values.
 $(\sum x)^2$ = square of the summation of the individual test values.

n = total number of test values

- 4.3 The lot standard deviation (s) is rounded to the nearest 0.01 for density and all sieve sizes except the 0.075 mm (No. 200) sieve. The lot standard deviation(s) is rounded to the nearest 0.001 for asphalt content and the 0.075 mm (No. 200) sieve.

NOTE 1: This is the sample standard deviation and not the population (sigma) standard deviation. Many computer spreadsheet programs have formulas for population standard deviation and not sample standard deviation.

- 4.4 Calculate the difference between the arithmetic mean (\bar{x}) and the lowest test result (X_L); and between the highest test result (X_H) and the arithmetic mean \bar{x}
- 4.5 Calculate test criterion, T_L or T_H , of the test result with the greatest difference from the arithmetic mean (\bar{x}).
- 4.6 If the lowest test result (X_L) has the greatest difference from the arithmetic mean \bar{x} , then T_L is calculated as follows:

$$T_L = \frac{(X_L - \bar{x})}{s}$$

- 4.1 If the highest test result (X_H) has the greatest difference from the arithmetic mean (\bar{x}), then T_H is calculated as follows:

$$T_H = \frac{(X_H - \bar{x})}{s}$$

Determine critical T value from Table 1.

- 4.2 If T_L or T_H , whichever is larger, exceeds the critical T value from Table 1, then that test result is an outlier and will be excluded from the price adjustment calculations. If one or more additional test result(s) has the same value as the outlier, then none of the test results will be outliers and all test results will be included in the price adjustment calculations. If T_L and T_H are equal, then neither test result will be an outlier and all test results will be included in the price adjustment calculations.

NOTE 2: This test method will not be reapplied to identify additional "outliers" based on the new arithmetic mean and sample standard deviations calculated after the "outliers" have been excluded.

Table 1
Critical T Values for a Sample Standard Deviation

Number Of Samples, n	Critical T
3	1.155
4	1.481
5	1.715
6	1.887
7	2.020
8	2.126
9	2.215
10	2.290
11	2.355
12	2.412
13	2.462
14	2.507
15	2.549
16	2.585
17	2.620

5. Example 1

1. Consider the following test results on percent asphalt content:

5.3, 5.6, 5.8, 5.8, 5.9, 5.9, 5.9, 6.0, 6.0 and 6.0

2. Calculate the arithmetic mean (\bar{x}) :

$$(\bar{x}) = \frac{5.3+5.6+5.8+5.8+5.9+5.9+5.9+6.0+6.0+6.0}{10}$$

$$(\bar{x}) = 5.82\%$$

3. Calculate the sample standard deviation:

$$s = \sqrt{\frac{n \sum (x^2) - (\sum x)^2}{n(n-1)}}$$

$$\begin{array}{rcl} \text{Where } \sum (x)^2 & = & 339.16 \\ (\sum x)^2 & = & 3,387.24 \\ n & = & 10 \\ s & = & 0.220 \end{array}$$

4. The difference between the arithmetic mean (\bar{x}) and the lowest test result is:

$$(5.82\% - 5.3\%) = 0.52\%$$

5. The difference between the highest test result and the arithmetic mean (\bar{x}) is:

$$(6.0\% - 5.82\%) = .18\%$$

6. Calculate T_L or T_H . Since the lowest test result (5.3%) had the greatest difference from the arithmetic mean (\bar{x}) it is evaluated to determine if it is an outlier. T_L is calculated as follows:

$$T_L = (5.82\% - 5.3\%) \div 0.220$$

$$T_L = 2.364$$

7. Determine Critical T. From Table 1, the critical T for 10 samples is 2.290. Since $T_L = 2.364$ is greater than 2.290, the test result of 5.3% is an outlier and is excluded from the price adjustment calculations.

6. Example 2

1. Consider the following test result on percent asphalt content:

5.3, 5.8, 5.8, 5.8, 5.9, 5.9, 6.0, 6.0, 6.0 and 6.5

2. Calculate arithmetic mean (\bar{x}):

$$x = \frac{5.3+5.8+5.8+5.8+5.9+5.9+6.0+6.0+6.0+6.5}{10}$$

$$x = 5.90\%$$

3. Calculate sample standard deviation:

$$s = \sqrt{\frac{n \sum (x^2) - (\sum x)^2}{n(n-1)}}$$

$$\begin{array}{rcl} \text{Where: } \sum (x)^2 & = & 348.88 \\ (\sum x)^2 & = & 3,481.00 \\ n & = & 10 \\ s & = & 0.294 \end{array}$$

4. The difference between the arithmetic mean x and the lowest test result is:

$$(5.90\% - 5.3\%) = 0.6\%$$

5. The difference between the highest test result and the arithmetic mean (\bar{x}) is:

$$(6.5\% - 5.90\%) = 0.6\%$$

6. Calculate T_L or T_H . Since the lowest test result (5.3%) and the highest test result (6.5%) have the same difference from the arithmetic mean (\bar{x}), both T_L and T_H are calculated.

$$T_L = (5.90\% - 5.3\%) \div 0.294$$

$$T_H = (6.5\% - 5.90\%) \div 0.294$$

$$T_L = T_H = 2.041$$

- 6.1.6 Since T_L and T_H are equal, neither test result is considered to be an outlier and all test results are included in the price adjustment calculation.

Standard Practice for Calibration of Pressure Type Air Meter SP 8

1. Scope

This practice covers the calibration of pressure type air meters used to determine the air content of freshly mixed concrete. Calibration procedures are developed to meet AASHTO T 152.

Note: This practice is equipment specific for two models of air meters currently in use by regional/field laboratories.

2. Apparatus

- Press-Ur-Meter (Charles R. Watts Company and Gilson)
- Appropriate calibration vessels for the air meters listed. Calibration vessels will have either be a vessel with an internal volume equal to 5 percent of the volume of the measuring bowl, or a vessel to place into the measuring bowl conforming to Note 1 in AASHTO T 152 and also equal to 5 percent. Regardless of type, the effective volume of the vessel should be checked.

3. Calibration Procedure for the Press-Ur-Meter:

- 3.1 Fill the measuring bowl with water.
- 3.2 Screw the straight tube into the threaded petcock hole on the underside of the cover. Clamp the cover assembly onto the measuring bowl with the tube extending down into the water.
- 3.3 With both petcocks open, add water through the petcock having the tubing extension, until all air is forced out the opposite petcock. Leave both petcocks open.
- 3.4 Pump air pressure to 0 percent or to the previous Initial Pressure line. Wait a few seconds for the compressed air to cool to ambient temperature, then stabilize the gauge needle at the assumed initial pressure by pumping up or bleeding off air, as necessary.
- 3.5 Close both petcocks and immediately press down on the air release lever exhausting the air into the measuring bowl. Wait a few seconds until the gauge needle is stabilized, tapping lightly on the gauge to keep gauge needle from sticking. If all the air was eliminated and the assumed Initial Pressure line was correct, the gauge should read 0 percent. If two or more tests show a consistent variation from 0 percent in the result, then change the Initial Pressure line to compensate for the variation, or remove the gauge glass and reset the gauge needle to 0 percent by turning the gauge's calibration screw. Use the newly established "Initial Pressure" line for subsequent tests.
- 3.6 Screw the curved tube into the outer end of the petcock with the straight tube below and, by pressing on the air release lever and controlling the flow with the petcock lever, fill the 5 percent calibrating vessel (345 ml) level full of water from the measuring bowl.
- 3.7 Release the air pressure at the free petcock. Open the other petcock and let the water in the curved pipe run back into the measuring bowl. There is now 5 percent air in the measuring bowl.
- 3.8 Pump air pressure to the Initial Pressure as determined in Step 5. Wait a few seconds for the compressed air to cool to ambient temperature and then stabilize the gauge needle at the assumed zero point by pumping up or bleeding off air, as necessary.
- 3.9 Close both petcocks and immediately press down on the air release lever exhausting the air into the measuring bowl. Wait a few seconds until the gauge needle is stabilized, tapping lightly on the gauge to keep gauge needle from sticking. If all the air was eliminated and the assumed Initial Pressure line was correct, the gauge should read 5 percent.
- 3.10 If two or more consistent tests show that the gauge at 5 percent air reads incorrectly in excess of 0.2

percent, then remove the gauge glass and reset the gauge needle to 5 percent by adjusting the gauge's calibration screw.

- 3.11 When the gauge reads correctly at 5 percent, additional water may be withdrawn in the same manner to check results at 10 percent.

4. Calibration Using Internal Calibration Vessel

- 4.1 Fill the measuring bowl with water.
- 4.2 Clamp the cover assembly onto the measuring bowl.
- 4.3 With both petcocks open, add water through one petcock, until all air is forced out the opposite petcock. Leave both petcocks open.
- 4.4 Pump air pressure to 0 percent or to the previous Initial Pressure Line. Wait a few seconds for the compressed air to cool to ambient temperature, then stabilize the gauge needle at the assumed zero point by pumping up or bleeding off air, as necessary.
- 4.5 Close both petcocks and immediately press down on the air release lever exhausting the air into the measuring bowl. Wait a few seconds until the gauge needle is stabilized, tapping lightly on the gauge to keep gauge needle from sticking. If all the air was eliminated and the assumed Initial Pressure line was correct, the gauge should read 0 percent. If two or more tests show a consistent variation from 0 percent in the result, then change the Initial Pressure line to compensate for the variation, or remove the gauge glass and reset the gauge needle to 0 percent by turning the gauge's calibration screw. Use the newly established "Initial Pressure" line for subsequent tests.
- 4.6 Release the pressure and remove the cover assembly.
- 4.7 Place the Internal Calibration Vessel into the measuring bowl, replace the cover assembly and refill as in step 3.
- 4.8 Pump the air pressure to the Initial Pressure Line allowing a few seconds for the gauge needle to stabilize.
- 4.9 Verify there is water standing in both petcocks and then close them.
- 4.10 Release to air into the measuring bowl by pressing down on the air release lever. Tap the gauge lightly and when stable, the meter should read 5 percent. If two or more consistent tests show that the gauge at 5 percent air reads incorrectly in excess of 0.2 percent, then remove the gauge glass and reset the gauge needle to 5 percent by adjusting the gauge's calibration screw and re-check.

5. Report

- 5.1 Report the results of the calibration as well as noting any adjustments or repairs made.
- 5.2 Label the meter with a sticker noting the month and year of the calibration.

Worksheets with Examples SP 10

1. Scope

- This standard practice includes copies of all the standard forms developed for use on DOT&PF projects. Examples have been included to help clarify their use.



STATE OF ALASKA
DOT & PF

FOP for T 180 Modified Proctor
FIELD WORKSHEET

☐ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____

AKSAS No: _____

Material: _____

Source: _____

Item No: _____

Location: _____

Sampled by / Qualification No: _____

Date: _____

Qty. Represented: _____

Standard Density — Modified Proctor — WAQTC FOP for T 180							METHOD:		Gradation, % Pass	
COMPACTION TEST	1	2	3	4	5	6			50mm / 2"	
A Mass of Mold									37.5mm / 1 1/2"	
B Mass of Mold + Wet Soil									25mm / 1"	
M Mass of Wet Sample B - A									19mm / 3/4"	
MOISTURE CONTENT — WAQTC FOP for T 255 / T 265							*W = [(Mw - Md) / Md] x 100		12.5mm / 1/2"	
C Container									9.5mm / 3/8"	
D Container + Moist Sample									4.75mm / #4	
Mw Moist sample D - C									2.36mm / #8	
E Container + Dry Sample									1.18mm / #16	
MD Dry Sample E - C									.600mm / #30	
*W Moisture Content, %									.300mm / #50	
Pw Wet Density									.150mm / #100	
Pd Dry Density									.075mm / #200	

ZAV Curve Calculations:

$$W_s = \frac{(62.4)(G_{sa}) - (Y_d)}{(Y_d)(G_{sa})} \times 100$$

Dry Density (Yd) Input for ZAV Curve: _____

Ws % Water Content for complete saturation

1 _____ 2 _____

F Factor: [1/(1/Mold Volume)] = _____

Mold Volume = _____

Pw Wet Density = (M x F)

Pd Dry Density = Pw / [1 + (W / 100)]

SPECIFIC GRAVITY — WAQTC FOP for T 85


b	SSD Aggregate Mass	
c	Aggregate Weight in Water	
a	Dry Aggregate Mass	
Gsb	BULK Specific Gravity = a / (b - c)	
	SSD Specific Gravity = b / (b - c)	
Gsa	Apparent Specific Gravity = a / (a - c)	
	Absorption = [(b - a) / a] x 100	

MAXIMUM DENSITY (0.1 lb/ft³ or 1 kg/m³) _____

OPTIMUM MOISTURE (0.1%) _____

Remarks: _____

DRY DENSITY vs. MOISTURE CONTENT

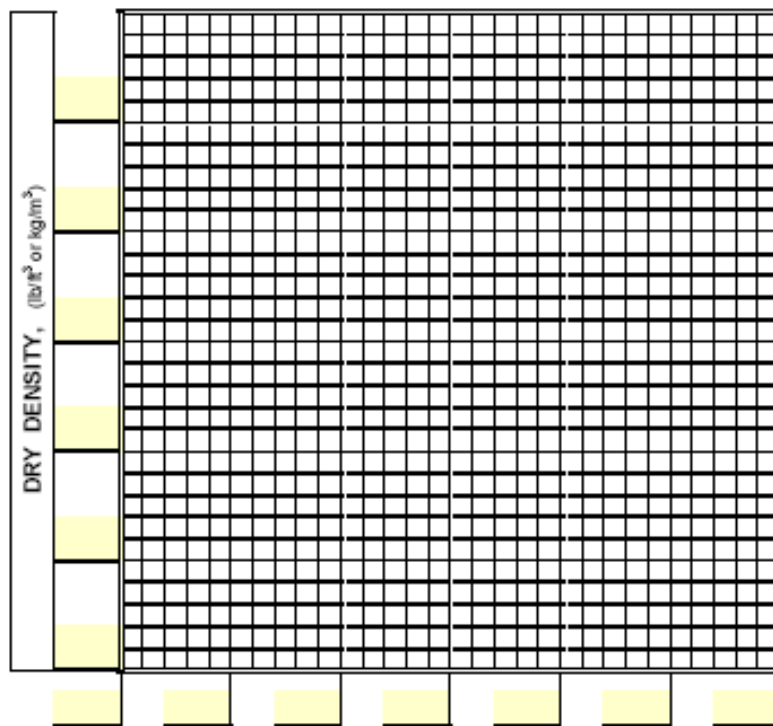

MOISTURE CONTENT, (%)

Tested by / Date: _____

Checked by / Date: _____



STATE OF ALASKA
DOT & PF

FOP for T 180 Modified Proctor
FIELD WORKSHEET

☐ Acceptance ☐ Verification ☐ Info. ☒ 1A ☐ QC

Sample No: 05C-119

Project Name: JNU EGAN DR / 10TH STREET INTERSECTION

Federal No: NH-093-2(29)

AKSAS No: 70168

Material: BEDDING MATERIAL

Source: MONTANA CREEK

Item No: 603

Location: JUNEAU, ALASKA

Sampled by / Qualification No: V. BEAN #079

Date: 4/5/2005

Qty. Represented: SOURCE

Standard Density — Modified Proctor — WAQTC FOP for T 180							METHOD: <input checked="" type="checkbox"/> D		Gradation, % Pass	
COMPACTION TEST										
A	Mass of Mold	12.61	12.61	12.61	12.61	12.61			50mm / 2"	
B	Mass of Mold + Wet Soil	23.08	23.35	23.52	23.71	23.88			37.5mm / 1 1/2"	
M	Mass of Wet Sample B - A	10.47	10.74	10.91	11.10	11.27			25mm / 1"	100
MOISTURE CONTENT — WAQTC FOP for T 255 / T 265							$^*W = [(M_w - M_d) / M_d] \times 100$		19mm / 3/4"	99
C	Container	522.1	544.6	546.1	567.8	538.8			12.5mm / 1/2"	80
D	Container + Moist Sample	848.8	955.0	852.2	913.1	894.6			9.5mm / 3/8"	69
Mw	Moist sample D - C	326.7	410.4	306.1	345.3	355.8			4.75mm / #4	51
E	Container + Dry Sample	840.0	942.0	838.5	896.9	876.5			2.36mm / #8	42
MD	Dry Sample E - C	317.9	397.4	292.4	329.1	337.7			1.18mm / #16	33
*W	Moisture Content, %	2.8	3.3	4.7	4.9	5.4			.600mm / #30	24
Pw	Wet Density	139.6	143.2	145.4	148.0	150.2			.300mm / #60	15
Pd	Dry Density	135.8	138.6	138.9	141.0	142.6			.150mm / #100	9
									.075mm / #200	5.2

ZAV Curve Calculations:

$$W_s = \frac{(62.4) (G_{sa}) - (P_d)}{(P_d) (G_{sa})} \times 100$$

Dry Density (Pd) Input for ZAV Curve:

7.0

9.0

W_s % Water Content for complete saturation

F Factor = 1 / Mold Volume = 13.33
Mold Volume Assumed = .0750

Pw Wet Density = (M x F)


Pd Dry Density = $P_w / [1 + (W / 100)]$

SPECIFIC GRAVITY — WAQTC FOP for T 85		
b	SSD Aggregate Mass	3052.8
c	Aggregate Weight in Water	1941.5
a	Dry Aggregate Mass	3027.7
Gsb	BULK Specific Gravity = $a / (b - c)$	2.725
	SSD Specific Gravity = $b / (b - c)$	2.747
Gsa	Apparent Specific Gravity = $a / (a - c)$	2.787
	Absorption = $[(b - a) / a] \times 100$	0.8

MAXIMUM DENSITY (0.1 lb/ft ³ or 1 kg/m ³)	141.0
OPTIMUM MOISTURE (0.1%)	5.0

Remarks: ALL IS WELL

DRY DENSITY vs. MOISTURE CONTENT

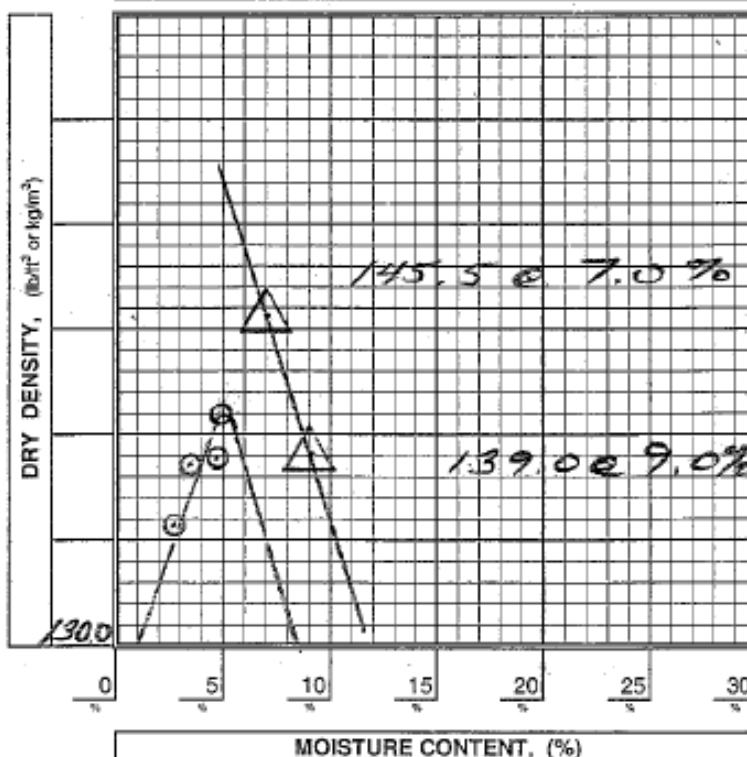

Tested by / Date: Jeffrey A. Hart / #009

Checked by / Date: Trinie Kelley / #041



STATE OF ALASKA
DOT & PF

**WAQTC FOP for T 310 (METHOD A)
FIELD DENSITY WORKSHEET**

☐ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Project Name:

Federal No:

AKSAS No:

Material:

Date:

Item No:

Spec:

Gauge S/N:

FIELD DENSITY TEST NUMBER				
STATION				
G_L REFERENCE				
GRADE REFERENCE				
QUANTITY REPRESENTED				
SOURCE				

STANDARD DENSITY		WAQTC FOP for T 180:		<input type="checkbox"/> A	<input type="checkbox"/> B	<input type="checkbox"/> C	<input type="checkbox"/> D	/	<input type="checkbox"/> ATM 212
Standard Density Lab Number									
Df Standard Density T 99/ T180 (Maximum Lab)									
Standard Density ATM 212 (from Chart)									
Optimum Moisture									
B Specific Gravity <input checked="" type="checkbox"/> Bulk <input type="checkbox"/> Apparent									

DENSITY DETERMINATION									
Probe Depth									
		Reading #1	Reading #2	Reading #1	Reading #2	Reading #1	Reading #2	Reading #1	Reading #2
Wet Density, (lb/ft ³ or kg/m ³)	Gauge								
C Average Wet Density									
Pd Dry Density (gauge)	$C / [1 + (E / 100)]$								
Dry Density (actual)	$C / [1 + (W / 100)]$								

MOISTURE CONTENT		<input type="checkbox"/> Use WAQTC FOP for T 255/T 265		<input type="checkbox"/> Use gauge moisture		<input type="checkbox"/> Use gauge moisture ONLY if within 1%			
% Moisture	Gauge								
E Average % Moisture									
F Wet Mass + Container									
G Dry Mass + Container									
J Container									
W % Moisture (actual)	$[(F - G) / (G - J)] \times 100$								

GRADATION / OVERSIZE CORRECTION		*Note: If % Oversize (Pc) is less than or equal to 5%, no correction is required.							
ATM 212 or *WAQTC FOP for T 224		<input type="checkbox"/> 3/4"	<input type="checkbox"/> #4	<input type="checkbox"/> 3/4"	<input type="checkbox"/> #4	<input type="checkbox"/> 3/4"	<input type="checkbox"/> #4	<input type="checkbox"/> 3/4"	<input type="checkbox"/> #4
P Wet Mass + Container									
Q Container									
Mm Wet Mass	P - Q								
Md Dry Mass	(actual) or $Mm / [1 + (E / 100)]$								
T Oversize Mass + Container									
V Container									
M _{oc} Oversize Mass	T - V								
Pc % Oversize	$(M_{oc} / Md) \times 100$								
Pf % Fines	$100 - Pc$								
Corrected Std. Density (Dd formula)									
% Compaction $(Pd / \text{Corr. Std. Den.}) \times 100$									
Dd = $(100 \times D_f k) / [(D_f \times Pc) + (k \times Pf)]$		$\Rightarrow k = (62.4 \text{ lb/ft}^3 \times B) \text{ or } (1000 \text{ kg/m}^3 \times B)$				TCTT = Too Coarse To Test			

Signature / Qualification No. / Date: _____ Checked by / Date: _____

REMARKS: _____



STATE OF ALASKA
DOT & PF

WAQTC FOP for T 310 (METHOD A)
FIELD DENSITY WORKSHEET

☒ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Project Name: Parks Hwy. Seward Meridian to Crusey

Federal No: NH-OA4-1(12)

AKSAS No: 52474

Material: Unclassified

Date: 7/12/2005

Item No:

Spec:

95%

Gauge S/N: 444888

FIELD DENSITY TEST NUMBER	SB-D-12			
STATION	122+00			
% _L REFERENCE	Lt 5'			
GRADE REFERENCE	Tob SB			
QUANTITY REPRESENTED	1/5000 cyd			
SOURCE	Existing			

STANDARD DENSITY

WAQTC FOP for T 180:

☐ A

☐ B

☐ C

☒ D

/

☐ ATM 212

Standard Density Lab Number	SB-SC-1			
Df Standard Density (Maximum Lab)	127.9			
Optimum Moisture	5.8			
B Bulk Specific Gravity	2.690			

DENSITY DETERMINATION

Probe Depth	8"								
		Reading #1	Reading #2	Reading #1	Reading #2	Reading #1	Reading #2	Reading #1	Reading #2
Wet Density, (lb/ft ³ or kg/m ³)	Gauge	137.9	139.1						
C Average Wet Density		138.5							
Pd Dry Density (gauge)	$C / [1 + (E / 100)]$	126.1							
Dry Density (actual)	$C / [1 + (W / 100)]$								

MOISTURE CONTENT

WAQTC FOP for T 255/T 265 or use gauge moisture if it is within 1% of actual moisture.

% Moisture	Gauge	9.8	9.8						
E Average % Moisture		9.8							
F Wet Mass + Container									
G Dry Mass + Container									
J Container									
W % Moisture (actual)	$[(F - G) / (G - J)] \times 100$								

GRADATION / OVERSIZE CORRECTION

*Note: If % Oversize (Pc) is less than or equal to 5%, no correction is required.

ATM 212 or *WAQTC FOP for T 224	<input checked="" type="checkbox"/> 3/4" <input type="checkbox"/> #4	<input type="checkbox"/> 3/4" <input type="checkbox"/> #4	<input type="checkbox"/> 3/4" <input type="checkbox"/> #4	<input type="checkbox"/> 3/4" <input type="checkbox"/> #4
P Wet Mass + Container	26.45			
Q Container	1.23			
Mm Wet Mass	P - Q	25.22		
Md Dry Mass	(actual) or $Mm / [1 + (E / 100)]$	22.97		
T Oversize Mass + Container	4.24			
V Container				
M _{oc} Oversize Mass	T - V	4.24		
Pc % Oversize	$(M_{oc} / Md) \times 100$	18		
Pf % Fines	100 - Pc	82		
Corrected Std. Density (Dd formula)		133.1		
Std. Density ATM 212 (from Chart)				
% Compaction	$(Pd / \text{Corr. Std. Den.}) \times 100$	95		

$$Dd = (100 \cdot D^p \cdot k) / [(Df \cdot Pc) + (k \cdot Pf)] \Rightarrow k = (82.4 \text{ lb/ft}^3 \cdot B) \text{ or } (1000 \text{ kg/m}^3 \cdot B)$$

Signature / Qualification No. / Date: J Dirks / 057 / 7-12-05

Checked by / Date:

REMARKS:



STATE OF ALASKA
DOT & PF

SOILS & AGGREGATE, METHOD A
FIELD WORKSHEET

☐ Acceptance ☐ Verification ☐ Info. ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____

AKSAS No: _____

Material: _____

Source: _____

Item No: _____

Location: _____

Sta. / Sampled from: _____

Sampled by / Qual. No: _____

C/L & Grade Reference: _____

Quantity Represented: _____

Date: _____

FRACTURE — WAQTC FOP for TP 61

<input checked="" type="checkbox"/> Single Face	<input type="checkbox"/> Double Face	<input type="checkbox"/> All Face
Fractured Mass F	% Q = $[Q / (F + Q + N)] \times 100$	
Questionable Mass Q	* % Questionable \Rightarrow _____	
Unfractured Mass N	* Recount if > 15%	
% Fracture	$\Leftarrow [F + (Q/2)] / (F + Q + N) \times 100$	
Test by/date: _____	\Leftarrow Spec. _____	

GRADATION — WAQTC FOP for T 27 / T 11 — Method A

mm / USC	Increment 1	Increment 2	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Specs.
75 / 3"						
50 / 2"						
37.5 / 1 1/2"						
25 / 1"						
19.0 / 3/4"						
12.5 / 1/2"						
9.5 / 3/8"						
6.3 / 1/4"						
4.75 / #4						
2.36 / #8						
2.00 / #10						
1.18 / #16						
.850 / #20						
.600 / #30						
.425 / #40						
.300 / #50						
.150 / #100						
.075 / #200						
Cum. Pan						
Cumulative Mass AFTER Sieving				\Leftarrow G	Check Sum (≤ 0.3%) $[(A - G) / A] \times 100 =$	
Dry Mass AFTER Wash BEFORE Sieving				\Leftarrow A	Test by/date: _____	
Original Dry Mass				\Leftarrow M		

MOISTURE CONTENT — WAQTC FOP for T 255 / T 265

C	Container	Constant Mass
A	Moist Mass + Container	Time _____ Gross Mass _____ Net Mass _____
Mw	Wet Mass A - C	
B	Dry Mass + Container	
Md	Dry Mass B - C	
W	Moisture, %	
W = $[(Mw - Md) / Md] \times 100$		% Change \Rightarrow _____
Test by/date: _____		% Change = $[(Mp - Mn) / Mp] \times 100$
Mp = Previous Mass Measured / Mn = New Mass Measured		

LIQUID AND PLASTIC LIMIT — WAQTC FOP for T 69 and T 90

	LL	PL
N	Number of Blows	
C	Container	
A	Moist Mass + Container	
Mw	Moist Mass A - C	
B	Dry Mass + Container	
Md	Dry Mass B - C	
W	Moisture Content, % $[(Mw - Md) / Md] \times 100$	
LL	W x (N / 25) ^{0.121}	
Test by/date: _____		
Plastic Index LL - PL		

FM \Rightarrow		\Leftarrow Fineness Modulus Target (From MD)
to		\Leftarrow FM Limits (± 0.2 of Mix Design FM)
(FM = Fineness Modulus = Total of % Retained of #Sieves / 100)		

Remarks:

Signature / Date: _____

Checked by / Date: _____



STATE OF ALASKA
DOT & PF

SOILS & AGGREGATE, METHOD A
FIELD WORKSHEET

☒ Acceptance ☐ Verification ☐ Info. ☐ QC

Sample No: Ex-G-1

Project Name: Parks Hwy. Seward meridian to Crusey

Federal No: NH-OA4-1(12)

AKSAS No: 52474

Material: Unclassified

Source: Existing

Item No: 203(3)

Location: Project Limits

Sta. / Sampled from: 304+10

Sampled by / Qual. No: J Dirks 057

C_L & Grade Reference: -9

Quantity Represented: as required

Date: 1/1/2006

FRACTURE — WAQTC FOP for TP 61			
<input checked="" type="checkbox"/> Single Face	<input type="checkbox"/> Double Face	<input type="checkbox"/> All Face	
Fractured Mass F	832.6	% Q = [Q / (F + Q + N)] x 100	
Questionable Mass Q	97.6	* % Questionable =>	9
Unfractured Mass N	352.3	* Recount if > 15%	
% Fracture	63	= [(F + (Q/2)) / (F + Q + N)] x 100	
Test by/date:	60	= Spec.	

MOISTURE CONTENT — WAQTC FOP for T 255 / T 265			
C	Container	1232.1	Constant Mass
A	Molst Mass + Container	2764.7	Time
			1:10
Mw	Wet Mass A - C	1532.6	1:45
			2:20
B	Dry Mass + Container	2633.1	
Md	Dry Mass B - C	1401.0	
W	Moisture, %	9	
W = [(Mw - Md) / Md] x 100		% Change =>	0.07
Test by/date:		% Change = [(Mp - Mn) / Mp] x 100	
Mp = Previous Mass Measured / Mn = New Mass Measured			

LIQUID AND PLASTIC LIMIT — WAQTC FOP for T 89 and T 90			
N	Number of Blows	23	PL
C	Container	14.20	14.18
A	Molst Mass + Container	24.22	23.69
Mw	Molst Mass A - C	10.02	9.51
B	Dry Mass + Container	22.63	22.61
Md	Dry Mass B - C	8.63	8.63
W	Moisture Content, %	16.1	10.2
LL	W x (N / 25) ^{0.121}	16	35
Test by/date:		Plastic Index LL - PL	6

Remarks:

GRADATION — WAQTC FOP for T 27 / T 11 — Method A						
mm / USC	Increment 1	Increment 2	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Specs.
"75 / 3"						
50 / 2"						
"37.5 / 1 1/2"						
25 / 1"						
"19.0 / 3/4"					100	
12.5 / 1/2"	724.7		724.7	14.0	86	
"9.5 / 3/8"	619.2		1343.9	26.0	74	
6.3 / 1/4"						
"4.75 / #4	1189.8		2533.7	49.0	51	
"2.36 / #6	877.6		3411.3	66.0	34	
2.00 / #10						
"1.18 / #16	574.8		3986.1	77.1	23	
.850 / #20						
".600 / #30	329.8		4315.9	83.5	16	
.425 / #40						
".300 / #50	228.5		4544.4	87.9	12	
".150 / #100	205.7		4750.1	91.9	8	
.075 / #200	135.4		4885.5	94.5	5.5	
Cum. Pan	20.4		4905.9	= G		Check Sum: (≤ 0.3%)
Cumulative Mass AFTER Sieving						[(A - G) / A] x 100 =
Dry Mass AFTER Wash BEFORE Sieving			4911.3	= A		0.11%
Original Dry Mass			5168.7	= M		Test by/date:

FM =>	4.81	4.70	= Fineness Modulus Target (From MD)
4.5	to	4.9	= FM Limits (± 0.2 of Mix Design FM)
(FM = Fineness Modulus = Total of % Retained of "Sieves / 100)			

Signature / Date:

Checked by / Date:



STATE OF ALASKA
DOT & PF

SOILS & AGGREGATE, METHOD B
FIELD WORKSHEET

☐ Acceptance ☐ Verification ☐ Info. ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____

AKSAS No: _____

Material: _____

Source: _____

Item No: _____

Location: _____

Sta. / Sampled from: _____

Sampled by / Qual. No: _____

G/L & Grade Reference: _____

Quantity Represented: _____

Date: _____

FRACTURE — WAQTC FOP for TP 61

<input checked="" type="checkbox"/> Single Face	<input type="checkbox"/> Double Face	<input type="checkbox"/> All Face
Fractured Mass F		% Q = $Q / (F + Q + N) \times 100$
Questionable Mass Q		* % Questionable \Rightarrow
Unfractured Mass N		* Recount if > 15%
% Fracture		$\Rightarrow (F + (Q/2)) / (F + Q + N) \times 100$
Test by/date		\Rightarrow Spec.

MOISTURE CONTENT — WAQTC FOP for T 255 / T 265

C	Container	Constant Mass
A	Moist Mass + Container	Time
Mw	Wet Mass A - C	Gross Mass
B	Dry Mass + Container	Net Mass
Md	Dry Mass B - C	
W	Moisture, %	
W = $[(Mw - Md) / Md] \times 100$		% Change \Rightarrow
Test by/date: _____		% Change = $[(Mp - Mn) / Mp] \times 100$
Mp = Previous Mass Measured / Mn = New Mass Measured		

LIQUID AND PLASTIC LIMIT — WAQTC FOP for T 89 and T 90

	LL	PL
N	Number of Blows	
C	Container	
A	Moist Mass + Container	
Mw	Moist Mass A - C	
B	Dry Mass + Container	
Md	Dry Mass B - C	PL
W	Moisture Content, % $[(Mw - Md) / Md] \times 100$	
LL	$W \times (N / 25)^{0.121}$	LL Spec.
Test by/date: _____		PI Spec.
Plastic Index LL - PL		

Remarks: _____

GRADATION — WAQTC FOP for T 27 / T 11 — Method B

mm / USC	Increment 1	Increment 2	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Specs.
75 / 3"						
50 / 2"						
37.5 / 1 1/2"						
25 / 1"						
19.0 / 3/4"						
12.5 / 1/2"						
9.5 / 3/8"						
6.3 / 1/4"						
4.75 / #4						
Pan				\Rightarrow M1	QA Check Sum ($\leq 0.3\%$)	
Cumulative Mass AFTER Sieving = (D + M1)				\Rightarrow G	$[(A - G) / A] \times 100 =$	
Dry Mass AFTER Wash BEFORE Sieving				\Rightarrow A		
Original Dry Mass				\Rightarrow M	Test by/date: _____	
				$\Rightarrow F = (M1 / M2) (0.001)$		

mm / USC	Cumulative Mass B	Total Sample Cumulative Mass C = [F x B] + D	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Specs.
2.36 / #8					
2.00 / #10					
1.18 / #16					
.850 / #20					
.600 / #30					
.425 / #40					
.300 / #50					
.150 / #100					
.075 / #200					
Cum. Pan P					
M2 \Rightarrow		\Rightarrow #4 Mass Actually Sieved		FA Check Sum ($\leq 0.3\%$)	
		Test by/date: _____		$[(M2 - P) / M2] \times 100 =$	

FM \Rightarrow		\Rightarrow Fineness Modulus Target (From MD)
to		\Rightarrow FM Limits (± 0.2 of Mix Design FM)
(FM = Fineness Modulus = Total of % Retained of *Sieves / 100)		

Signature / Date: _____

Checked by / Date: _____



STATE OF ALASKA
DOT & PF

SOILS & AGGREGATE, METHOD B
FIELD WORKSHEET

☒ Acceptance ☐ Verification ☐ Info. ☐ QC

Sample No: Ex-G-1

Project Name: Parks Hwy. Seward meridian to Cruise

Federal No: NH-OA4-1(12)

AKSAS No: 52474

Material: Unclassified

Source: Existing

Item No: 203(3)

Location: Project Limits

Sta. / Sampled from: 304+10

Sampled by / Qual. No: J Dirks 057

C/L & Grade Reference: -9

Quantity Represented: as required

Date: 1/12/2006

FRACTURE — WAQTC FOP for TP 61			
<input checked="" type="checkbox"/> Single Face	<input type="checkbox"/> Double Face	<input type="checkbox"/> All Face	
Fractured Mass F	632.6	% Q = $(Q / (F + Q + N)) \times 100$	
Questionable Mass Q	97.6	* % Questionable \Rightarrow	9
Unfractured Mass N	352.3	* Recount if > 15%	
% Fracture	63	$\Leftarrow (F + (Q/2)) / (F + Q + N) \times 100$	
Test by/date:	60%	\Leftarrow Spec.	

MOISTURE CONTENT — WAQTC FOP for T 255 / T 265			
C	Container	1232.1	Constant Mass
A	Moist Mass + Container	2764.7	Time
Mw	Wet Mass A - C	1532.6	1:10
B	Dry Mass + Container	2633.1	1:45
Md	Dry Mass B - C	1401.0	2:20
W	Moisture, %	9	% Change \Rightarrow
W = $((Mw - Md) / Md) \times 100$		0.07	
Test by/date:		% Change = $((Mp - Mn) / Mp) \times 100$	
Mp = Previous Mass Measured / Mn = New Mass Measured			

LIQUID AND PLASTIC LIMIT — WAQTC FOP for T 69 and T 90			
N	Number of Blows	23	PL
C	Container	14.20	14.18
A	Moist Mass + Container	24.22	23.69
Mw	Moist Mass A - C	10.02	9.51
B	Dry Mass + Container	22.83	22.81
Md	Dry Mass B - C	8.63	8.63
W	Moisture Content, %	16.1	10.2
LL	W x $(N / 25)^{0.121}$	16	35
Test by/date:		Plastic Index	10
		LL - PL	12

Remarks:

GRADATION — WAQTC FOP for T 27 / T 11 — Method B						
mm / USC	Increment 1	Increment 2	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Specs.
"75 / 3"						
50 / 2"						
"37.5 / 1 1/2"						
25 / 1"						
"19.0 / 3/4"					100	
12.5 / 1/2"	161.1		161.1	5.0	95	
"9.5 / 3/8"	481.4		642.5	20.0	80	
6.3 / 1/4"						
"4.75 / #4	475.8		1118.3	34.8	65	
Pan	1966.7		1966.7	\Leftarrow M1		
Cumulative Mass AFTER Sieving = (D + M1)			3085.0	\Leftarrow G		
Dry Mass AFTER Wash BEFORE Sieving			3085.1	\Leftarrow A		
Original Dry Mass			3214.0	\Leftarrow M		
3.835			\Leftarrow F = (M1 / M2) (0.001)			

mm / USC	Cumulative Mass B	Total Sample Cumulative Mass C = (F x B) + D	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Specs.
"2.36 / #8					
2.00 / #10	207.1	1912.6	59.5	41	
"1.18 / #16					
.850 / #20					
"600 / #30					
.425 / #40	395.0	2633.2	81.9	18	
".300 / #50					
".150 / #100	454.9	2862.9	89.1	11	
.075 / #200	504.0	3051.3	94.9	5.1	
Cum. Pan P	511.8				
M2 \Rightarrow	512.8	\Leftarrow #4 Mass Actually Sieved			
Test by/date:					

FM \Rightarrow		\Leftarrow Fineness Modulus Target (From MD)
to		\Leftarrow FM Limits (± 0.2 of Mix Design FM)
(FM = Fineness Modulus = Total of % Retained of "Sieves / 100)		

Signature / Date:

Checked by / Date:



STATE OF ALASKA
DOT & PF

SOILS & AGGREGATE, METHOD C
FIELD WORKSHEET

☐ Acceptance ☐ Verification ☐ Info. ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____

AKSAS No: _____

Material: _____

Source: _____

Item No: _____

Location: _____

Sta. / Sampled from: _____

Sampled by / Qual. No: _____

C/L & Grade Reference: _____

Quantity Represented: _____

Date: _____

FRACTURE — WAQTC FOP for TP 61

<input type="checkbox"/> Single Face	<input type="checkbox"/> Double Face	<input type="checkbox"/> All Face
Fractured Mass F		% Q = $[Q / (F + Q + N)] \times 100$
Questionable Mass Q		* % Questionable \Rightarrow _____
Unfractured Mass N		* Recount if > 15%
% Fracture		$\Rightarrow [F + (Q/2)] / (F + Q + N) \times 100$
Test by/date: _____		\Rightarrow Spec. _____

GRADATION — WAQTC FOP for T 27 / T 11 — Method C

mm / USC	Increment 1	Increment 2	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Specs.
100 / 4"						
"75 / 3"					t	
50 / 2"						
"37.5 / 1 1/2"						
25 / 1"						
"19.0 / 3/4"						
12.5 / 1/2"						
"9.5 / 3/8"						
6.3 / 1/4"						
"4.75 / #4						
Pan				\Rightarrow M1	CA Check Sum ($\leq 0.3\%$)	
Dry Mass AFTER Sieving = (D + M1)				\Rightarrow G	$[M - G] / M \times 100 =$	
Original Dry Mass BEFORE Sieving				\Rightarrow M		
				$\Rightarrow F = (M1 / M3) (0.001)$	Test by/date: _____	

MOISTURE CONTENT — WAQTC FOP for T 255 / T 265

C	Container	Constant Mass
A	Moist Mass + Container	Time _____ Gross Mass _____ Net Mass _____
Mw	Wet Mass A - C	
B	Dry Mass + Container	
Md	Dry Mass B - C	
W	Moisture, %	
$W = [(Mw - Md) / Md] \times 100 \%$		% Change \Rightarrow _____
Test by/date: _____		% Change = $[(Mp - Mn) / Mp] \times 100$
Mp = Previous Mass Measured / Mn = New Mass Measured		

LIQUID AND PLASTIC LIMIT — WAQTC FOP for T 69 and T 90

	LL	PL
N	Number of Blows	\times
C	Container	
A	Moist Mass + Container	
Mw	Moist Mass A - C	
B	Dry Mass + Container	
Md	Dry Mass B - C	PL
W	Moisture Content, % $[(Mw - Md) / Md] \times 100$	
LL	$W \times (N / 25)^{0.121}$	LL Spec.
Test by/date: _____	Plastic Index LL - PL	PI Spec.

Remarks: _____

mm / USC	Cumulative Mass B	Total Sample Cumulative Mass C = (F x B) + D	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Specs.
"2.36 / #8					
2.00 / #10					
"1.18 / #16					
.850 / #20					
" .600 / #30					
.425 / #40					
" .300 / #50					
" .150 / #100					
.075 / #200					
Cum. Pan P		#200 on - 3" = $[(s / t) \times 100] \Rightarrow$			
H \Rightarrow		\Rightarrow Total Mass AFTER Wash		FA Check Sum ($\leq 0.3\%$)	
M3 \Rightarrow		\Rightarrow - #4 Mass BEFORE Wash		$[(H - P) / H] \times 100 =$	
		Test by/date: _____			

FM \Rightarrow		\Rightarrow Fineness Modulus Target (From MD)
	to	\Rightarrow FM Limits (± 0.2 of Mix Design FM)
(FM = Fineness Modulus = Total of % Retained of *Sieves / 100)		

Signature / Date: _____

Checked by / Date: _____



STATE OF ALASKA
DOT & PF

SOILS & AGGREGATE, METHOD C
FIELD WORKSHEET

☒ Acceptance

☐ Verification

☐ Info.

☐ QC

Sample No: Ex-G-1

Project Name: Parks Hwy. Seward meridian to Crusey

Federal No: NH-OA4-1(12)

AKSAS No: 58474

Material: Unclassified

Source: Existing

Item No: 203(3)

Location: Project Limits

Sta. / Sampled from: 304+10

Sampled by / Qual. No: J Dirks 057

ϕ_L & Grade Reference: -9

Quantity Represented: as required

Date: 1/12/2006

FRACTURE — WAQTC FOP for TP 61			
<input checked="" type="checkbox"/> Single Face	<input type="checkbox"/> Double Face	<input type="checkbox"/> All Face	
Fractured Mass F	832.8	% Q = $[(F + Q + N) / (F + Q + N)] \times 100$	
Questionable Mass Q	97.6	* % Questionable \Rightarrow	9
Unfractured Mass N	352.3	*Recount if > 15%	
% Fracture	83	$\Rightarrow [(F + Q) / (F + Q + N)] \times 100$	
Test by/date:		80% \Rightarrow Spec.	

MOISTURE CONTENT — WAQTC FOP for T 255 / T 265			
C	Container	1232.1	Constant Mass
A	Moist Mass + Container	2784.7	Time
MW	Wet Mass A - C	1532.6	1:10
B	Dry Mass + Container	2833.1	1:45
Md	Dry Mass B - C	1401.0	2:20
W	Moisture, %	9	
W = $[(Mw - Md) / Md] \times 100$		% Change \Rightarrow	0.07
Test by/date:		% Change = $[(Mp - Mn) / Mp] \times 100$	
Mp = Previous Mass Measured / Mn = New Mass Measured			

LIQUID AND PLASTIC LIMIT — WAQTC FOP for T 69 and T 90			
		LL	PL
N	Number of Blows	23	
C	Container	14.20	14.18
A	Moist Mass + Container	24.22	23.69
MW	Moist Mass A - C	10.02	9.51
B	Dry Mass + Container	22.83	22.81
Md	Dry Mass B - C	8.63	8.63
W	Moisture Content, %	16.1	10.2
LL	W x (N / 25) ^{0.121}	16	
Test by/date:		Plastic Index	6
		LL - PL	
		LL Spec.	
		PI Spec.	

Remarks:

GRADATION — WAQTC FOP for T 27 / T 11 — Method C						
mm / USC	Increment 1	Increment 2	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Specs.
100 / 4"						
75 / 3"						
50 / 2"						
37.5 / 1 1/2"						
25 / 1"						
19.0 / 3/4"					100	
12.5 / 1/2"	125.9		125.9	3.8	96	
9.5 / 3/8"	478.2		604.1	18.3	82	
6.3 / 1/4"						
4.75 / #4	691.5		1295.6	39.1	61	
Pan	2008.9		2008.9	\Rightarrow M1	CA Check Sum ($\leq 0.3\%$)	
Dry Mass AFTER Sieving = (D + M1)			3304.5	\Rightarrow G	$[(M - G) / M] \times 100 =$	
Original Dry Mass BEFORE Sieving			3310.0	\Rightarrow M	0.2%	
			3.808	\Rightarrow F = (M1 / M3) (0.001)	Test by/date:	

mm / USC	Cumulative Mass B	Total Sample Cumulative Mass C = (F x B) + D	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Specs.
2.36 / #8					
2.00 / #10	194.3	2035.4	61.5	39	
1.18 / #16					
.850 / #20					
.600 / #30					
.425 / #40	365.6	2687.7	81.2	19	
.300 / #50					
.150 / #100	430.8	2935.9	88.7	11	
.075 / #200	484.4	3140.0	94.9	5	5.0
Cum. Pan P	495.1	#200 on - 3" = $[(s / t) \times 100] \Rightarrow$			
H \Rightarrow	495.3	\Rightarrow Total Mass AFTER Wash		FA Check Sum ($\leq 0.3\%$)	
M3 \Rightarrow	527.6	\Rightarrow #4 Mass BEFORE Wash		$[(H - P) / H] \times 100 =$	
Test by/date:					

FM \Rightarrow		\Rightarrow Fineness Modulus Target (From MD)
to		\Rightarrow FM Limits (± 0.2 of Mix Design FM)
(FM = Fineness Modulus = Total of % Retained of *Sieves / 100)		

Signature / Date:

Checked by / Date:



**STATE OF ALASKA
DOT & PF**

**AGGREGATE, Sand Equivalent
FIELD WORKSHEET**

☐ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____

AKSAS No: _____

Material: _____

Source: _____

Item No: _____

Location: _____

Sta. / Sampled from: _____

Sampled by: _____

C/L & Grade Reference: _____

Qualification No: _____

Date Sampled: _____

Sand Equivalent WAQTC FOP T 176			
Sedimentation Time		20 min.	
Trial No.	1	2	3
Sand Reading SR			
Clay Reading CR			
Sand Equivalent SE			
Sedimentation Time			
$SE = (SR / CR) * 100$			
Test by/date:		Average	

Flat and Elongated ATM 305						
Ratio: <input type="checkbox"/> 1:5 <input type="checkbox"/> 1:3 <input type="checkbox"/> 1:2						
Size Fraction	mm	Group % Retained (A)	Dry Mass	F & E Mass	% F & E (B)	Weighted % F&E (C)
37.5 to 19.0	1½ to ¾					
19.0 to 9.5	¾ to ¾					
9.5 to 4.75	¾ to No. 4					
(A) Group Retained is based on plus No. 4 only				Total Weighted %		
(B) % F & E = [(F & E Mass) / (Dry Mass)] * 100				Test by/date: _____		
(C) Weighted % F & E = Group % Retained / % F & E						

Remarks: _____

Signature / Date: _____

Checked by / Date: _____

Rev.3/31/06



**STATE OF ALASKA
DOT & PF**

**AGGREGATE, Sand Equivalent
FIELD WORKSHEET**

☐ Acceptance ☐ Verification ☒ Info. ☐ IA ☐ QC

Sample No: SE LAB #05C-383

Project Name: Ketchikan Tongass Avenue Resurfacing

Federal No: IM-0902(28)

AKSAS No: 68140

Material: Asphalt Conc., SP, Type A

Source: Glacier Northwest

Item No: 401(1)

Location: Dupont, WA

Sta. / Sampled from:

Sampled by: WA

C/L & Grade Reference:

Qualification No: 1202

Date Sampled: 6/4/2005

Sand Equivalent WAQTC FOP T 176			
Sedimentation Time		20 min.	
Trial No.	1	2	3
Sand Reading SR	4.1	4.3	4.1
Clay Reading CR	6.3	6.7	6.5
Sand Equivalent SE	66	65	64
Sedimentation Time	20 min.	20 min	20 min
SE = (SR / CR) * 100			
Test by/date:		Average	65

Flat and Elongated ATM 306							
Ratio: <input checked="" type="checkbox"/> 1:5 <input type="checkbox"/> 1:3 <input type="checkbox"/> 1:2							
Size Fraction	mm	Group % Retained (A)	Dry Mass	F & E Mass	% F & E (B)	Weighted % F&E (C)	
37.5 to 19.0	1 1/2 to 3/4						
19.0 to 9.5	3/4 to 3/8	12.5	695.4	10.5	2	2	
9.5 to 4.75	3/8 to No. 4	10.2	158.9	6.3	4	2	
(A) Group Retained is based on plus No. 4 only				Total Weighted %		4	
(B) % F & E = [(F & E Mass) / (Dry Mass)] * 100				Test by/date:			
(C) Weighted % F & E = Group % Retained / % F & E							

Remarks:

Signature / Date:

Checked by / Date:



STATE OF ALASKA
DOT & PF

HMA Extracted Aggregate Gradation
FOP for T 30 - FIELD WORKSHEET

☐ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____ AKSAS No: _____

Material: _____ Source: _____

Item No: _____ Location: _____

Sta. / Sampled from: _____ Sampled by / Qual. No: _____

C_L & Grade Reference: _____ Quantity Rep'd: Lot _____ Sublot # _____ Date/Time: _____

FRACTURE — WAQTC FOP for TP 61

☐ Single Face ☐ Double Face ☐ All Face

Fractured Mass	F	* % Questionable ⇒ * Recount if > 15%
Questionable Mass	Q	
Unfractured Mass	N	
% Fracture		$\Rightarrow \frac{F + (Q/2)}{F + Q + N} \times 100$

Test by/date: _____ Spec. _____

MOISTURE CONTENT — WAQTC FOP for T 255 / T 265

C	Container	Constant Mass
A	Moist Mass + Container	Time
Mw	Wet Mass A - C	Grav Mass
B	Dry Mass + Container	Net Mass
Md	Dry Mass B - C	
W	Moisture, %	

$W = \frac{Mw - Md}{Md} \times 100$ if % Change = _____

Test by/date: _____ % Change = $\frac{[Mp - Mn] / Mp}{[Mp - Mn] / Mp} \times 100$

Mp = Previous Mass Measured / Mn = New Mass Measured

LIQUID AND PLASTIC LIMIT — WAQTC FOP for T 89 and T 90

	LL	PL
N	Number of Blows	
C	Container	
A	Moist Mass + Container	
Mw	Moist Mass A - C	
B	Dry Mass + Container	
Md	Dry Mass B - C	
W	Moisture Content, % $\frac{[Mw - Md]}{Md} \times 100$	
LL	W x (N / 25) ^{0.121}	35

Test by/date: _____ Plastic Index LL - PL _____ 6 PL Spec.

Remarks: _____

HMA AGGREGATE GRADATION — WAQTC FOP for T 30

mm / USC	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	***Aggregate Correction	Reported % Passing	Specs.
50 / 2"				Add Subtract		—
*37.5 / 1 1/2"						—
25 / 1"						—
*19.0 / 3/4"						—
12.5 / 1/2"						—
*9.5 / 3/8"						—
6.3 / 1/4"						—
*4.75 / #4						—
*2.36 / #8						—
2.00 / #10						—
*1.18 / #16						—
.850 / #20						—
*.600 / #30						—
.425 / #40						—
*.300 / #50						—
*.150 / #100						—
.075 / #200			*			—
Pan (only)		⇐ P	* #200 = $\frac{[(M - A) + P]}{M} \times 100$			

Cumulative Mass AFTER Sieving ⇐ G Test by/date: _____

Dry Mass AFTER Wash BEFORE Sieving ⇐ A

**Dry Sample Mass before Wash ⇐ M ** (within 0.1% of Mf FOP for T 308)

☐ Wetting Agent Used

Check Sum (< 0.2%)

$\frac{[A - G]}{A} \times 100 =$

** (M) must be within 0.1% of (Mf)

Dry Sample Mass before Wash (M) = _____ % of mass of aggregate remaining after ignition FOP for T 308

Mf 1933.1

***For aggregate correction to adjust sieves correctly, you must input numbers from the HMA Correction Factors Worksheet. Use minus sign in subtract column. Enter 0 in column if no adjustment.

FM ⇐ _____ ⇐ Fineness Modulus Target (From MD)

to _____ ⇐ FM Limits (± 0.2 of Mix Design FM)

(FM = Fineness Modulus = Total of % Retained of *Sieves / 100)

Copy to Contractor/Date: _____

Tested By / Qual#: _____

Signature / Date: _____

Checked by / Date: _____



STATE OF ALASKA
DOT & PF

HMA Extracted Aggregate Gradation
FOP for T 30 - FIELD WORKSHEET

☐ Acceptance ☒ Verification ☐ Info. ☐ IA ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____

AKSAS No: _____

Material: _____

Source: _____

Item No: _____

Location: _____

Sta. / Sampled from: _____

Sampled by / Qual. No: _____

C/L & Grade Reference: _____

Quantity Rep'd: Lot _____

Sublot # _____

Date/Time: _____

FRACTURE — WAQTC FOP for TP 61			
<input type="checkbox"/> Single Face	<input type="checkbox"/> Double Face	<input type="checkbox"/> All Face	
Fractured Mass F	1088.0	% Q = $[Q / (F + Q + N)] \times 100$	5
Questionable Mass Q	67.0	* % Questionable \Rightarrow	
Unfractured Mass N	277.0	*Recount if > 15%	
% Fracture	78	$= [(F + (Q/2)) / (F + Q + N)] \times 100$	
Test by/date:			\Leftarrow Spec.

MOISTURE CONTENT — WAQTC FOP for T 255 / T 265			
C	Container	1232.1	Constant Mass
A	Moist Mass + Container	2764.7	Time
			Green Mass
			Net Mass
			1:10
			1405.1
Mw	Wet Mass A - C	1532.6	1:45
			2634.1
B	Dry Mass + Container	2633.1	2:20
			1402.0
Md	Dry Mass B - C	1401.0	
			2633.1
W	Moisture, %	9	
W = $[(Mw - Md) / Md] \times 100$		% Change \Rightarrow	0.07
Test by/date:		% Change = $[(Mp - Mn) / Mp] \times 100$	
Mp = Previous Mass Measured / Mn = New Mass Measured			

LIQUID AND PLASTIC LIMIT — WAQTC FOP for T 89 and T 90			
N	Number of Blows	23	LL
C	Container	14.20	PL
A	Moist Mass + Container	24.22	23.69
Mw	Moist Mass A - C	10.02	9.51
B	Dry Mass + Container	22.83	22.81
Md	Dry Mass B - C	8.63	8.63
W	Moisture Content, %	16.1	10.2
	$[(Mw - Md) / Md] \times 100$		
LL	W x (N / 25) ^{0.121}	16	35
Test by/date:	Plastic Index	6	6
	LL - PL		

Remarks: _____

HMA AGGREGATE GRADATION — WAQTC FOP for T 30						
mm / USC	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	***Aggregate Correction	Reported % Passing	Specs.
50 / 2"				Add		—
*37.5 / 1 1/2"						—
25 / 1"						—
*19.0 / 3/4"			100.0		100	—
12.5 / 1/2"	172.4	8.9	91.0		91	—
*9.5 / 3/8"	421.2	21.8	78.0		78	—
6.3 / 1/4"						—
*4.75 / #4	950.8	49.3	51.0		51	—
*2.36 / #8	1290.1	66.8	33.0		33	—
2.00 / #10						—
*1.18 / #16	1495.7	77.5	23.0		23	—
.850 / #20						—
*.600 / #30	1608.3	83.3	17.0		17	—
.425 / #40						—
*.300 / #50	1679.1	87.0	13.0		13	—
*.150 / #100	1731.0	89.7	10.0		10	—
.075 / #200	1779.9	92.2	* 7.8		7.8	—
Pan (only)	19.2	\Leftarrow P	* #200 = $[(M - A) + P] / M \times 100$			
Cumulative Mass AFTER Sieving			1799.1	\Leftarrow G	Test by/date:	
Dry Mass AFTER Wash BEFORE Sieving			1799.4	\Leftarrow A		
**Dry Sample Mass before Wash			1930.4	\Leftarrow M	** (within 0.1% of M FOP for T 308)	

<input type="checkbox"/> Wetting Agent Used		Check Sum ($\leq 0.2\%$)
** (M) must be within 0.1% of (Mf)		$[(A - G) / A] \times 100 =$
Dry Sample Mass before Wash (M) = 0.1 % of		0.0
mass of aggregate remaining after ignition FOP for T 308		
Mf	1933.1	

***For aggregate correction to adjust sieves correctly, you must input numbers from the HMA Correction Factors Worksheet. Use minus sign in subtract column. Enter 0 in column if no adjustment.

FM \Rightarrow		\Leftarrow Fineness Modulus Target (From MD)
	to	\Leftarrow FM Limits (± 0.2 of Mix Design FM)
(FM = Fineness Modulus = Total of % Retained of *Sieves / 100)		

Copy to Contractor/Date: _____

Tested By / Qual#: _____

Signature / Date: _____

Checked by / Date: _____



STATE OF ALASKA
DOT & PF

HMA Correction Factors
FIELD WORKSHEET

☐ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____ AKSAS No: _____

Material: _____ Agg. Source: _____

Item No: _____ Location: _____

WAQTC FOP for T 308, Method: _____ Mix Design No.: _____ Furnace No. / ID: _____

ASPHALT CEMENT CORRECTION					WAQTC FOP for T 308		CORRECTION FACTORS	AGGREGATE CORRECTION		Sample #1	Sample #2
Mix Design %AC #1		After Burn %AC #1		%AC Diff. #1		D		Sample & Basket Assembly			
Mix Design %AC #2		After Burn %AC #2		%AC Diff. #2		B		Basket Assembly			
Cf	AC CORRECTION FACTOR (average of differences)					Mf		Mass after Ignition (D-B)			

HMA AGGREGATE GRADATION				AGGREGATE CORRECTION					
WAQTC FOP for T 30				WAQTC FOP for T 308					
mm / USC	Correction Factor Blank Sample			Correction Factor Sample #1			Correction Factor Sample #2		
	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained
25 / 1"									
19.0 / 3/4"									
12.5 / 1/2"									
9.5 / 3/8"									
4.75 / #4									
2.36 / #8									
1.18 / #16									
.600 / #30									
.300 / #50									
.150 / #100									
.075 / #200									
Cum. Pan Mass			Check Sum ≤0.2			Check Sum ≤0.2			Check Sum ≤0.2
Dry Mass After Wash				Dry Mass After Wash			Dry Mass After Wash		
M Mass Before Wash				M Mass Before Wash			M Mass Before Wash		
									Calculate & Report % Passing to 0.1%

mm / USC	Allowable Difference	Blank Sample % Passing	Sample #1 % Passing	Sample #2 % Passing	Difference from Blank Sample		Average Difference	*Sieves to Adjust	
					#1	#2		Add	Subtract
25 / 1"	± 5.0 %								
19.0 / 3/4"	± 5.0 %								
12.5 / 1/2"	± 5.0 %								
9.5 / 3/8"	± 5.0 %								
4.75 / #4	± 5.0 %								
2.36 / #8	± 5.0 %								
1.18 / #16	± 3.0 %								
.600 / #30	± 3.0 %								
.300 / #50	± 3.0 %								
.150 / #100	± 3.0 %								
.075 / #200	± 0.5 %								

Adjust Sieves for FOP for T 30 Gradation: Use "0" if adjustment N/A; use minus sign for negative numbers in subtract column.

Remarks: _____

Signature / Date: _____
**Checked by / Date: _____



STATE OF ALASKA
DOT & PF

HMA Correction Factors
FIELD WORKSHEET

☐ Acceptance ☒ Verification ☐ Info. ☐ IA ☐ QC

Sample No: SE LAB #05C-383

Project Name: Ketchikan Tongass Avenue Resurfacing

Federal No: IM-0902(28)

AKSAS No: 68140

Material: Asphalt Conc., SP, Type A

Agg. Source: Glacier Northwest

Item No: 401(1)

Location: Dupont WA

WAQTC FOP for T 308, Method: A

Mix Design No.: O5C-383

Furnace No. / ID: JNU - SE Lab #1

ASPHALT CEMENT CORRECTION WAQTC FOP for T 308						AGGREGATE CORRECTION			Sample #1	Sample #2
Mix Design %AC #1	5.3	After Burn %AC #1	5.8	%AC Diff. #1	0.5	D	Sample & Basket Assembly		5389.6	5418.8
Mix Design %AC #2	5.3	After Burn %AC #2	5.9	%AC Diff. #2	0.6	B	Basket Assembly		3315.6	3343.7
Cf	AC CORRECTION FACTOR (average of differences)				0.5	Mf	Mass after Ignition (D-B)		2074.0	2075.1

HMA AGGREGATE GRADATION WAQTC FOP for T 30				AGGREGATE CORRECTION WAQTC FOP for T 308					
mm / USC	Correction Factor Blank Sample			Correction Factor Sample #1			Correction Factor Sample #2		
	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained	Cumulative Mass Retained C	Cumulative % Retained (C / M) x 100	% Passing = 100 - % Retained
25 / 1"	0.0	0.0	100.0	0.0	0.0	100.0	0.0	0.0	100.0
19.0 / 3/4"	169.9	8.1	91.9	153.3	7.4	92.6	168.1	8.1	91.9
12.5 / 1/2"	663.9	31.8	68.4	587.1	28.3	71.7	575.9	27.7	72.3
9.5 / 3/8"	1026.1	48.9	51.1	970.8	46.8	53.2	981.1	47.3	52.7
4.75 / #4	1305.2	62.2	37.8	1280.6	61.7	38.3	1279.6	61.6	38.4
2.36 / #8	1579.1	75.2	24.8	1552.5	74.8	25.2	1559.0	75.1	24.9
1.18 / #16	1740.3	82.9	17.1	1718.6	82.8	17.2	1724.0	83.0	17.0
.600 / #30	1844.3	87.8	12.2	1825.0	88.0	12.0	1831.0	88.2	11.8
.300 / #50	1908.7	90.9	9.1	1887.6	91.0	9.0	1894.7	91.3	8.7
.150 / #100	1947.7	92.7	7.3	1926.7	92.9	7.1	1933.9	93.2	6.8
.075 / #200	1988.6	94.70	5.30	1966.9	94.82	5.18	1975.5	95.16	4.84
Cum. Pan Mass	2002.5	0.0	Check Sum <0.2	1991.0		Check Sum <0.2	1991.8		Check Sum <0.2
Dry Mass After Wash	2002.6			1995.0			1992.1		
M	Mass Before Wash	2100.0	M	Mass Before Wash	2074.4	M	Mass Before Wash	2076.0	Calculate & Report % Passing to 0.1%

mm / USC	Allowable Difference	Blank Sample % Passing	Sample #1 % Passing	Sample #2 % Passing	Difference from Blank Sample		Average Difference	*Sieves to Adjust	
					#1	#2		Add	Subtract
25 / 1"	± 5.0 %	100.0	100.0	100.0	0.0	0.0	0.0	0.0	0.0
19.0 / 3/4"	± 5.0 %	91.9	92.6	91.9	-0.7	0.0	-0.3	0.0	0.0
12.5 / 1/2"	± 5.0 %	68.4	71.7	72.3	-3.3	-3.9	-3.6	0.0	0.0
9.5 / 3/8"	± 5.0 %	51.1	53.2	52.7	-2.1	-1.6	-1.9	0.0	0.0
4.75 / #4	± 5.0 %	37.8	38.3	38.4	-0.5	-0.6	-0.6	0.0	0.0
2.36 / #8	± 5.0 %	24.8	25.2	24.9	-0.4	-0.1	-0.2	0.0	0.0
1.18 / #16	± 3.0 %	17.1	17.2	17.0	-0.1	0.1	0.0	0.0	0.0
.600 / #30	± 3.0 %	12.2	12.0	11.8	0.2	0.4	0.3	0.0	0.0
.300 / #50	± 3.0 %	9.1	9.0	8.7	0.1	0.4	0.3	0.0	0.0
.150 / #100	± 3.0 %	7.3	7.1	6.8	0.2	0.5	0.4	0.0	0.0
.075 / #200	± 0.5 %	5.30	5.18	4.84	0.12	0.46	0.29	0.00	0.00

Remarks:

Signature / Date: Jeff Hart #009 8/1/05

**Checked by / Date: TK 8/2/05



STATE OF ALASKA
DOT & PF

STANDARD DENSITY by CONTROL STRIP
ATM 412 - FIELD WORKSHEET

☐ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____

AKSAS No: _____

Material: _____

Source: _____

Item No: _____

Gauge Model: _____

Gauge S/N: _____

Standard Count: _____

Station to Station: _____

Lane: _____

Width: _____

Date: _____

**All initial readings are to be Wet Density 15 Second readings and taken in backscatter position.*

Equipment	Pass #:	*Site 1	*Site 2	*Site 3	Average	Change	Remarks / Temp.					
<u>Drum Roller</u> Roller Brand: _____ Model No: _____ Frequency (VPM): _____ Amplitude: _____	1					X						
	2											
	3											
	4											
	5											
<u>Pneumatic Roller</u>	1					X						
	2											
	3											
	4											
	5											
Locations ⇒		1	2	3	4	5	6	7	8	9	10	
Reading 1 (1 minute)												Standard Density
Reading 2 (1 minute)												
Average Wet Density												
Moisture control is not required for HMA or ATB												
Reading 1 % Moisture												Average Moisture
Reading 2 % Moisture												
Average % Moisture												

Remarks: _____

Tested By / Qualification No: _____

Signature / Date: _____

Checked by / Date: _____



STATE OF ALASKA
DOT & PF

STANDARD DENSITY by CONTROL STRIP
ATM 412 - FIELD WORKSHEET

☒ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Sample No: _____

Project Name: _____

Federal No: _____

AKSAS No: _____

Material: _____

Source: _____

Item No: _____

Gauge Model: _____

Gauge S/N: _____

Standard Count: _____

Station to Station: _____

Lane: _____

Width: _____

Date: _____

**All initial readings are to be Wet Density 15 Second readings and taken in backscatter position.*


Equipment	Pass #:	*Site 1	*Site 2	*Site 3	Average	Change	Remarks / Temp.				
<u>Drum Roller</u>	1	127.3	130.3	126.2	127.9	XXXX					
Roller Brand: _____	2	131.2	134.1	132.7	132.7	4.8					
Model No: _____	3	133.3	133.2	135.1	133.9	1.2					
Frequency (VPM): _____	4	132.7	132.4	135.6	133.6	-0.3					
Amplitude: _____	5										
<u>Pneumatic Roller</u>	1	135.5	137.1	131.1	134.6	XXXX					
	2	138.9	136.4	134.8	136.7	2.1					
	3										
	4										
	5										
Locations ⇒	1	2	3	4	5	6	7	8	9	10	
Reading 1 (1 minute)	135.1	133.4	134.1	137.2	130.1	135.3	137.5	134.9	133.6	139.7	Standard Density
Reading 2 (1 minute)	137.2	134.3	133.8	138.9	129.2	136.5	139.8	132.1	131.7	141.3	
Average Wet Density	136.2	133.9	134.0	138.1	129.7	135.9	138.7	133.5	132.7	140.5	
Moisture control is not required for HMA or ATB											
Reading 1 % Moisture											Average Moisture
Reading 2 % Moisture											
Average % Moisture											

Remarks: _____

Tested By / Qualification No: _____

Signature / Date: _____

Checked by / Date: _____



STATE OF ALASKA
DOT & PF
Density and Depth
FIELD WORKSHEET - WAQTC TM 8

☐ Info. ☐ QC

Sample No: _____

Federal No: _____ AKSAS No: _____ Gauge & Model No: _____

Material: _____ Source: _____ Serial No: _____

Item No: _____ Density Standard: 154 *Correlation Factor: _____ Spec: _____

LOCATION and Area Represented: _____ Qty Represented: _____ Core Set No: _____ Date: _____

FIELD DENSITY TEST NUMBER	1	2	3	4	5	6	7	8	9	10
STATION										
C/L REFERENCE (offset)										
GRADE REFERENCE										
QUANTITY REPRESENTED										
DENSITY DETERMINATION <input type="checkbox"/> Backscatter Mode										
(Reading #2 is rotated 90° from reading #1)	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2
D Wet Density, lb/ft ³ (Difference <= 2.5 (b/f))										
E Average Wet Density										
F Adj Density (use *Correlation Factor)										
G % Compaction (F / Density Std) x 100										
CORRELATION with CORES										
WAQTC POP for AASHTO T 166	Core 1	Core 2	Core 3	Core 4	Core 5	Core 6	Core 7	Core 8	Core 9	Core 10
H Core Thickness (inches)										
A Mass of Dry Specimen in Air										
B Mass of SSD Specimen in Air										
C Weight of Specimen in Water										
J Bulk Specific Gravity (.001) A / (B - C)										
K Unit Wt = Bulk SpG x 62.4 (pcf)										
E Avg Wet Density (from E above)										
L Difference = Unit Wt - Avg Wet Density K - E										

☐ Filler Material (Native Fines) Used

Tested by / Qualif: _____

Avg Difference: _____


REMARKS : _____

Signature / Date: _____

Standard Deviation (<= 2.5): _____

Checked by / Date: _____

Rev.12/31/05



**STATE OF ALASKA
DOT & PF**

Density and Depth

FIELD WORKSHEET - WAQTC TM 8

☐ Acceptance ☐ Verification ☒ Info ☐ IA ☐ QC

Federal No: STPOL9-998 AKSAS No: 92541

Material: Asphalt Conc., SP, Type A Source: Glacier Northwest

Item No: 401(1) Density Standard: 157.3 *Correlation Factor: _____

Sample No: XX-XX-352

Gauge & Model No: XXXXX/3430

Serial No: XXXXXXXX

Spec: 92-98%

Date: 7/4/2005

LOCATION and Area Represented: _____ Test Strip _____ Qty Represented: _____ Core Set No: _____

FIELD DENSITY TEST NUMBER	1	2	3	4	5	6	7	8	9	10
STATION	12+80	16+44	18+12	20+95	22+45	24+20	26+88	28+36	30+99	32+48
C/L REFERENCE (offset)	8' Lt	7' Rt	4' Rt	12' Lt	5' Lt	2' Lt	8' Rt	11' Rt	7' Rt	3' Lt
GRADE REFERENCE										
QUANTITY REPRESENTED										

DENSITY DETERMINATION ☒ Backscatter Mode

(Reading #2 is rotated 90° from reading #1)		Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2	Reading #1 / Reading#2
D	Wet Density, lb/ft ³ (Difference <=2.5 lb/ft ³)	151.2	152.0	150.3	150.6	151	153	151.6	152.9	152.6	151.6
		150.9	151.3	151	150.1	150.9	152.4	152	152.6	152.3	151.1
E	Average Wet Density	151.1	151.7	150.7	150.4	151	152.7	151.8	152.8	152.5	151.4
F	Adj Density (use *Correlation Factor)										
G	% Compaction (F / Density Std) x 100	96.1	96.4	95.8	95.6	96	97.1	96.5	97.1	96.9	96.2

CORRELATION with CORES

WAQTC POP for AASHTO T 166	Core 1	Core 2	Core 3	Core 4	Core 5	Core 6	Core 7	Core 8	Core 9	Core 10
H Core Thickness (inches)	2	2	2	2	2	2	2	2	2	2
A Mass of Dry Specimen in Air	1647.6	1795.4	1895.4	1859.2	1844.3	1649.7	1651.9	1655.8	1659.7	1670.1
B Mass of SSD Specimen in Air	1651.2	1799.4	1898.1	1863.8	1846.6	1652.7	1655.3	1658.3	1664.4	1672.9
C Weight of Specimen in Water	986.5	1084.9	990.6	977.6	984.1	978.2	974.3	978.6	980.5	983
J Bulk Specific Gravity (.001) A / (B - C)	2.406	2.444	2.396	2.418	2.409	2.446	2.426	2.436	2.427	2.421
K Unit Wt = Bulk SpG x 62.4 (pcf)	150.1	152.5	149.5	150.9	150.3	152.6	151.4	152.0	151.4	151.1
E Avg Wet Density (from E above)	151.1	151.7	150.7	150.4	151	152.7	151.8	152.8	152.5	151.4
L Difference = Unit Wt - Avg Wet Density K - E	-1.0	0.8	-1.2	0.5	-0.7	-0.1	-0.4	-0.8	-1.1	-0.3

☐ Filler Material (Native Fines) Used

Tested by / Qual# : xyz No. 00022221 Avg Difference: -0.4

REMARKS : _____

Signature / Date: _____ Standard Deviation (<= 2.5): 0.67

Checked by / Date: _____

Rev. 12/31/05



STATE OF ALASKA
DOT & PF

CONCRETE PLACEMENT REPORT
FIELD WORKSHEET

☐ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Pour No: _____

Project Name: _____

Federal No: _____

AKSAS No: _____

Date: _____

Structure / Bridge: _____

Item No: _____

Stations / Area Rep'd: _____

Truck No: _____

Supplier: _____

Class: _____

Ticket No: _____

Aggregate Source: _____

Cement/Type: _____

Mix Design No: _____

BATCH MASS (from Scale)

Lbs.

Nt	Cementitious Material (Nc + Nf + Nm)			
Port. Cem. (Nc)		Fly Ash (Nf)		M-silica (Nm)
A	Fine Aggregate or Sand (FA)			
B	Intermediate Aggregate (IA)			
C	Coarse Aggregate (CA)			
D	Water Added at Plant		gal. x 8.34 lbs. ⇒	
D1	Water Added on Site		gal. x 8.34 lbs. ⇒	
W1	Total Mass of Batch (Nt + A + B + C + D + D1)			

AGGREGATE SSD WEIGHTS

FA	a	Free Moisture, %		-		%
	b	SSD Weight $[A / (1 + (a / 100))]$	(% Moisture)*	(absorption)**		
IA	c	Free Moisture, %		-		%
	d	SSD Weight $[B / (1 + (c / 100))]$	(% Moisture)*	(absorption)**		
CA	e	Free Moisture, %		-		%
	f	SSD Weight $[C / (1 + (e / 100))]$	(% Moisture)*	(absorption)**		

* Moisture From Batch Ticket

** Absorption From Mix Design, use 0.0% if Batch Ticket reports free moisture

MASS OF WATER IN BATCH

Lbs.

E	Free Water in FA (A - b)	
F	Free Water in IA (B - d)	
G	Free Water in CA (C - f)	
H	Total Water Mass (D + D1 + E + F + G)	

Pour Time: Start		Finish	
Mix Time:		Mix Revs:	
Time of Discharge:			
Spec. = 1 1/2 hrs. with +1 minute per degree < 70°F, not to exceed 2 hrs.			
Time Between Batches:		< 30 Minutes	

TEMPERATURE — WAQTC FOP for T 309

Concrete Temperature		Weather Conditions	
Air Temperature			
Water Temperature			

WAQTC FOP for:

Specs:

T 119	Slump, in.		
T 152	Air, %		
a	Mass of Bucket + Conc.		lb.
b	Mass of Bucket		lb.
Mm	Mass of Conc. (a - b)		lb.
Vm	Bucket Volume		ft ³
W	T 121 Density (Mm/Vm)		lb / ft ³
Test by/date: _____			

CYLINDER DATA — WAQTC FOP for T 23

Time Made		Cylinder ID	
Spec:			
Test by/date: _____			

Yd ³ Batch Design	BATCH DATA		Actual yd ³ Batch Data	Specifications	Allowable Range*
VB	Design Batch Volume, nearest 0.01 yd ³				
	Actual yd ³ / Batch = $W1 / (27 \times W)$, nearest 0.01 yd ³	YB		* excludes 608, 609, 615, & Aviation items	
	Yield per yd ³ Batch = YB / VB , nearest 0.01 yd ³	Y			
W / C	Water Cement Ratio (lb / lb) = H / Nt , nearest 0.01	W / C			
Mix Design Proportions	Cementitious Content (lb / yd ³) = Nt / YB , nearest lb.	N		± 1%	Batch Design
	Sacks / yd ³ = $N / 94$, nearest 0.1 sack				
	Portland Cement Content (lb / yd ³) = Nc / YB , nearest lb.			± 1%	Batch Design
	Fly Ash Content (lb / yd ³) = Nf / YB , nearest lb.			± 5%	Batch Design
	Microsilica Content (lb / yd ³) = Nm / YB , nearest lb.			± 10%	Batch Design
	Fine Aggregate = b / YB , nearest lb.			± 2%*	Batch Design
	Intermediate Aggregate = d / YB , nearest lb.			± 2%*	Batch Design
	Coarse Aggregate = f / YB , nearest lb.			± 2%*	Batch Design

Remarks: _____

Signature / Date: _____

Checked by / Date: _____

Rev.1/31/06



STATE OF ALASKA
DOT & PF

CONCRETE PLACEMENT REPORT
FIELD WORKSHEET

☒ Acceptance ☐ Verification ☐ Info. ☐ IA ☐ QC

Pour No: A 1 - Load #1

Project Name: Egan Drive/10th St. Intersection Improvements, Phase 1

Federal No: NH-F-093-2(29)

AKSAS No: 70188

Date: 8/8/2005

Structure / Bridge: Curb and Gutter Standard

Item No: 809(2a)

Stations / Area Rep'd: "G" 2+00, Lt. To "D" 7+00, Lt.

Truck No: 9

Supplier: AggPro

Class: A

Ticket No: 4576

Aggregate Source: Glacier Northwest

Cement/Type: Ash Grove Type I-II

Mix Design No: 05C-130

BATCH MASS (from Scale)					Lbs.
Nt	Cementitious Material (Nc + Nf + Nm)				2491
Port. Cem. (Nc)	2094	Fly Ash (Nf)	397	M-silica (Nm)	
A	Fine Aggregate or Sand (FA)				5489
B	Intermediate Aggregate (IA)				
C	Coarse Aggregate (CA)				7804
D	Water Added at Plant	79	gal. x 8.34 lbs. ⇨		659
D1	Water Added on Site	11	gal. x 8.34 lbs. ⇨		92
W1	Total Mass of Batch (Nt + A + B + C + D + D1)				16535

AGGREGATE SSD WEIGHTS				
FA	a	Free Moisture, %	4.2	4.20 %
	b	SSD Weight $[A / (1 + (a / 100))]$ (% Moisture)*		5288 (absorption)**
IA	c	Free Moisture, %		%
	d	SSD Weight $[B / (1 + (c / 100))]$ (% Moisture)*		0 (absorption)**
CA	e	Free Moisture, %	1.70	1.70 %
	f	SSD Weight $[C / (1 + (e / 100))]$ (% Moisture)*		7674 (absorption)**

* Moisture From Batch Ticket

** Absorption From Mix Design, use 0.0% if Batch Ticket reports free moisture

MASS OF WATER IN BATCH				Lbs.
E	Free Water in FA (A - b)			221
F	Free Water in IA (B - d)			0
G	Free Water in CA (C - f)			130
H	Total Water Mass (D + D1 + E + F + G)			1102

Pour Time: Start	10:54 AM	Finish	12:05 PM
Mix Time:	Mix Revs:	Time of Discharge:	
10 Min	70	11:45 AM	
Spec. = 1 1/2 hrs. with +1 minute per degree < 70°F, not to exceed 2 hrs.			
Time Between Batches:	1st load	< 30 Minutes	

TEMPERATURE — WAQTC FOP for T 309			
Concrete Temperature	68	Weather Conditions	
Air Temperature	65	Partly Cloudy	
Water Temperature	59	No Rain or Wind	

WAQTC FOP for:				Specs:
	T 119	Slump, in.	4	2"-4"
	T 152	Air, %	5.0%	4-7%
a	Mass of Bucket + Conc.		43.75	lb.
b	Mass of Bucket		7.89	lb.
Mm	Mass of Conc. (a - b)		38.06	lb.
Vm	Bucket Volume		0.2494	ft ³
W	T 121	Density (Mm/Vm)	144.6	lb / ft ³
Test by/date:		V. Bean #079 / 6-8-05		

CYLINDER DATA — WAQTC FOP for T 23			
Time Made	Cylinder ID		
11:30 AM	1	5210	
Spec: 4000 psi	2	5120	
Test by date:		VB 6-8-05	

Yd ³ Batch Design	BATCH DATA			Actual yd ³ Batch Data	Specifications	Allowable Range*
4.25	VB	Design Batch Volume, nearest 0.01 yd ³				
		Actual yd ³ / Batch = $W1 / (27 \times W)$, nearest 0.01 yd ³	YB	4.24	* excludes 608, 609, 615, & Aviation items	
		Yield per yd ³ Batch = YB / VB , nearest 0.01 yd ³	Y	1.00		
0.45	W / C	Water Cement Ratio (lb / lb) = H / Nt , nearest 0.01			W / C	0.44
		Cementitious Content (lb / yd ³) = Nt / YB , nearest lb.	N	588	± 1%	Batch Design
		Sacks / yd ³ = $N / 94$, nearest 0.1 sack		6.3		
494		Portland Cement Content (lb / yd ³) = Nc / YB , nearest lb.		494	± 1%	Batch Design
94		Fly Ash Content (lb / yd ³) = Nf / YB , nearest lb.		94	± 5%	Batch Design
		Microsilica Content (lb / yd ³) = Nm / YB , nearest lb.			± 10%	Batch Design
1250		Fine Aggregate = b / YB , nearest lb.		1242	± 2%*	Batch Design
		Intermediate Aggregate = d / YB , nearest lb.			± 2%*	Batch Design
1800		Coarse Aggregate = f / YB , nearest lb.		1810	± 2%*	Batch Design

Remarks: Air entrainment added at 6 oz/cy Mix

Signature / Date:

Design = 6 oz/cy, No WRA

Checked by / Date:

Rev. 1/31/06

Contractor Quality Control SP 11

1. Scope

This standard practice covers basic tasks and procedures Contractors working on Alaska Department of Transportation and Public Facilities (DOT&PF) Highway and Airport Construction projects are to follow. This Standard is required only when it is specified for the project and the minimum quantities as shown in the Introductions of the various materials are met. These procedures are intended for the development and successful operation of the Contractor's Quality Control Plan (QCP).

Quality Control/Quality Assurance (QC/QA) is often used synonymously with the term Quality Assurance (QA). AASHTO defines Quality Assurance as: "All those planned and systematic actions necessary to provide confidence that a product will perform satisfactorily in service." This definition considers that QA is an all encompassing concept that includes process control or quality control, acceptance, and independent assurance (IA).

The DOT&PF further defines the QC/QA process by differentiating the duties of the Contractor and the DOT&PF. The Contractor is responsible for all quality and process control (QC) activities. The DOT&PF is responsible for all activities involved in acceptance of the material and for independent assurance (IA). These separate activities are intended to work together in order to provide the public a well performing project.

Refer to SP-1 and the Alaska Test Methods (ATM) Manual in general for further definitions of terms and acronyms used in this Standard Practice.

2. Services Furnished By Contractor

Provide a QC Laboratory with an office area that is separate from the Engineer's field office/laboratory to safely: keep personnel; house testing equipment; run testing equipment; maintain calibrated testing equipment; calibrate testing equipment; perform testing and; keep records in with telephone and email access. Specific lists of equipment and calibration requirements are contained in tables in Sections 5.0 to 9.0. Also provide a QC curing shed to properly cure concrete samples, separate from the Engineer's, when it is required for the project. See AASHTO R 18, Establishing and Implementing a Quality Management System for Construction Materials Testing Laboratories for guidelines. Any QC Laboratory and QC Curing Shed set up for a particular project is considered part of the project's work site or work area.

3. Quality Control Organization

Implement the QCP by establishing a quality control organization (QCO) with authority to ensure compliance with the contract plans and specifications, and authority to halt construction until deficiencies are corrected. None of the QCO may be employed by those performing acceptance activities on the project.

Develop an organizational chart showing all quality control personnel and how these personnel integrate with other management/production and construction functions and personnel. Provide phone numbers for all parties within the quality control organization.

Include the names, qualifications, telephone number, duties, and employer of all quality control personnel necessary to implement the QCP. Minimum QCO functions are as follows.

- 3.1 The QCP Plan Administrator (PA) is the person responsible for the overall administration of the QCP. The PA must have full authority to institute actions necessary for successful implementation of the QCP, including ensuring compliance with the contract plans and specifications, and halting construction until deficiencies are corrected. The PA reports directly to a responsible officer of the construction firm. The PA may supervise the QCP on more than one project provided that person can be contacted by phone within two hours and will be at the job site within 24 hours after being notified of a problem. The PA is a full-time employee of the Contractor, or an independent consultant hired by the Contractor with experience on projects of comparable size and scope as in the current QCP. Additional qualifications of the PA include at least one of the following.
- a) Professional Engineer in Alaska with at least one year of construction experience acceptable to the Engineer.
 - b) Engineer-in-Training with at least two years of construction experience acceptable to the Engineer.
 - c) An individual with at least three years of construction experience acceptable to the Engineer, with a Bachelor of Science Degree in Civil Engineering, Civil Engineering Technology or Construction.
 - d) An individual with at least five years experience in quality control activities in highway or airport construction on projects of similar size and scope as in the current QCP.
 - e) Construction materials technician WAQTC qualified and with experience on projects of comparable size and scope acceptable to the Engineer in performing all tests used in the QCP.
 - f) Construction materials technician, Highway materials technician or, Highway construction technician certified at Level III by the National Institute for Certification in Engineering Technologies (NICET).
 - g) A NICET certified engineering technician in Civil Engineering Technology with 5 years of experience acceptable to the Engineer.
- 3.2 Quality Control Technician(s) are the person(s) responsible for conducting quality control inspection, sampling and testing to adequately implement the QCP and control the construction activities. Provide sufficient qualified QC personnel as required to monitor each work activity at all times including plant and field inspectors. Additional requirements for QC Technicians are as follows.
- a) Effective January 1, 2010, WAQTC Qualified Technicians in each area of their work. American Concrete Institute (ACI) field testing technician, grade 1 is acceptable for Concrete testing requirements.
 - b) QC Technicians report directly to the PA.
 - c) The QC Technicians are responsible for field inspection, sampling and testing of all materials and maintaining all testing equipment in accordance with the QCP and contract specifications.
 - d) QC Technicians must have at least two years experience in their area of inspection, sampling and testing on projects of similar size and scope as addressed in the current QCP.

4. General Quality Control Plan Requirements

Include the following items in the Contractor's Quality Control Plan (QCP):

- 4.3 Make the QCP contract specific, stating how the Contractor proposes to control the materials, equipment, and construction operations including subcontractors and suppliers as well as production facilities and transportation modes to the project.
- 4.1 Identify all applicable AASHTO, ASTM, ATM and WAQTC and any other referenced standards in the QCP.
- 4.2 Use the QCP to ensure conformance to the contract and DOT&PF Specifications with respect to materials, workmanship, construction, and finish.
- 4.3 Identify, locate and provide access for any laboratories, curing sheds or other locations where QC testing and any other QC work is planned.
- 4.4 State in the QCP that the Engineer has unrestricted access to the Laboratory, and all QC test results at any time. The Engineer may observe QC testing in the Laboratory or the field and may report any inconsistencies in the implementation of the QCP to the Contractor's Plan Administrator for resolution. All findings are to be resolved within 24 hours of notification.
- 4.5 Submit the QCP to the Engineer at least as many days as shown in the contract specifications prior to the Preconstruction Conference and be prepared to discuss the QCP at that meeting. Have the QCP signed and dated by the Contractor's Project Superintendent at the time it is submitted to the Engineer.
- 4.6 The Engineer will review, sign, and date the QCP if the contents of the QCP are in compliance with the requirements as stated herein. Provide a copy of the signed QCP to the Engineer. Do not begin any construction until the QCP has been signed by the Engineer.
- 4.7 Maintain the QCP to reflect the current status of the operations, and provide any revisions in writing for the Engineer to review per section 4.7. Modification requests to the QCP must include:
 - a) Revised pages in the QCP noting the changes and the effective date of change;
 - b) Signed by the Plan Administrator;
 - c) Submit any revisions related to certified materials, QCP material control limits, QCP material testing equipment, Contractor's Organization and/or, change in QCO for review;.
 - d) Revisions related to contractor processes, construction phasing, etc., may be discussed verbally with the Engineer as long as it is documented in an Appendix of the QCP.
- 4.8 The Contractor is responsible for all QC documentation and submitting a copy of all the documentation to the Engineer at the completion of the project. This documentation does not include methods or tests outside of those that are defined herein that a contractor wants to keep as a trade secret.
- 4.9 Have a testing plan in the QCP that identifies the minimum tests to be completed, proposed methods of sampling, frequency of testing, calibration of test equipment, construction control and monitoring activities to adequately control the production and construction processes.

4.10 **Control Charts.** Include the procedures for creating and maintaining control charts of the QC results. Include as minimum, the following:

- a) Create Control Charts that identify the project number, the contract number, the item number, test numbers, test parameters, target value (if applicable), action and suspension limits. Plot test results applicable to each test parameter.
- b) Place target values, if applicable, in the center of the chart represented by a horizontal heavy long dash followed by a short dash line.
- c) Place and identify control limits on the chart represented by heavy solid lines.
- d) Indicate full payment limits short dashed lines.
- e) Make the vertical range of control charts between upper and lower control limits no less than two (2) inches in height allowing for the entire range of expected test results.
- f) Make the plot points for the test results surrounded by a small circle with each consecutive point connected by a solid straight line.
- g) Plot the test results from left to right in chronological order, and show dates or test numbers corresponding to each test along the horizontal axis.
- h) Make at least one control chart for each type of test result that is taken. Define the data used on control charts: individual test points; moving averages and/or: test ranges for each chart
- i) Identify any proposed deviation from these instructions in the QCP.
- j) Keep all QC testing current, in accordance with the QCP with the results posted within 24 hours in the QC Laboratory. These may be made available on a computer in the Laboratory. Provide an email connection and printer connected to the computer so that results can be emailed or printed out for the Engineer upon request.
- k) Maintain files of all written documentation as factual evidence that testing was performed.

4.11 **Corrective Action Plans. Develop corrective action plans including stopping** rules for reacting to the various situations that could be demonstrated in the control charts, materials testing and field inspections. Have corrective actions that range from minor adjustments to temporarily stopping production/construction with immediate reactions depending on findings of the Quality Control Organization.

4.12 **Payment for materials.** No partial payment will be made for materials subject to specific quality control requirements until the QCP has been signed by the Engineer. Payment will only be made for materials that have completed quality control operations according to the QCP. Payment is not allowed for materials produced after test results are available that instigate the QCP stopping rules.

5. Quality Control of Earthwork Materials

5.1 Introduction. This section applies to fill materials without fracture requirements used on a project under Highway's Specification Division 200, Division 300 or Airport Technical Specifications for Earthwork. Contractor Quality Control processes as stated herein are required on DOT&PF projects that have contract quantities for individual pay items equal to or greater than 100,000 tons or 50,000 cubic yards. Then perform all quality control testing necessary to control the production and construction processes in accordance with a QCP developed per these standard practices.

5.2 Field Operating Procedures, Alaska Test Methods and Standard Practices listed below are those used for materials acceptance and are thus recommended for QC. Some of these tests are for quality of the materials that must be checked prior to production. Other tests may be proposed in the QCP subject to the Engineer's review.

a) WAQTC Field Operation Procedures (FOPs):

- FOP for AASHTO T 2 Sampling of Aggregates
- FOP for AASHTO T 248 Reducing Samples of Aggregate to Testing Size
- FOP for AASHTO T 255/T 265 Moisture Content of Aggregate and Soil
- FOP for AASHTO T 27/T 11 Sieve Analysis of Aggregates and Soils
- FOP for AASHTO T 99/T 180 Moisture-Density Relations of Soils
- FOP for AASHTO T 85 Specific Gravity and Absorption of Coarse Aggregate
- FOP for AASHTO T 224 Correction for Coarse Particles in the Soil Compaction Test
- FOP for AASHTO T 89 Determining the Liquid Limit of Soils
- FOP for AASHTO 90 Determining the Plastic Limit and Plasticity Index of Soils
- FOP for AASHTO T 310 In-Place Density and Moisture Content of Soil and Soil-Aggregate by Nuclear Methods (Shallow Depth)

b) Alaska Test Methods (ATMs) and Standard Practices (SPs)

- ATM 203 Organic Content of Soils by Ignition
- SP 1 Terminology
- SP 2 Calibration of Mechanical Compaction Hammer/Rammer
- SP 4 Random Sampling
- SP 6 Rounding and Precision in Materials Test Reporting
- SP 7 Determination of Outlier Test Results

5.3 **Testing Equipment.** Provide a list of the testing equipment proposed for quality control testing. List test methods the equipment is used for and the frequency of calibration or verification of the equipment. Maintain a record of all equipment calibration or verification results at the testing facility. The maximum intervals and procedures shall be as shown in the Table below.

SUMMARY OF EQUIPMENT REQUIRING CALIBRATION/VERIFICATION

Equipment *	Requirement	Max. Interval (Months)	Performed By:
Coarse Sieves (\geq #4 Sieve)	Check Openings and Physical Condition	6	Lab Personnel
Fine Sieves ($<$ #4 Sieve)	Check Physical Condition	6	Lab Personnel
Thermometers	Standardize	6	Lab Personnel
Timers	Check Accuracy	6	Lab Personnel
Ovens	Verify Temperature Settings	4	Lab Personnel
General Purpose Scales	Verify	12	Lab Personnel
Analytical Scales		12	
General Purpose Weights	Verify	12	Outside Agency
Analytical Weights		12	
Mechanical Shakers	Check Sieving Thoroughness	12	Lab Personnel
Manual Rammers	Check Mass & Critical Dimensions	12	Lab Personnel
Compaction Molds	Check Critical Dimensions	12	
Straight Edges	Check Plainness of Edge	6	
Mechanical Compactors	Check Mass & Critical Dimensions Calibrate vs. Manual Hammer	12	
Coarse SpG	Verify Operator Proficiency	6	Lab Personnel
Liquid Limit Devices & Grooving Tools	Check Wear & Critical Dimensions	12	Lab Personnel
Nuclear Density Gauges	Calibrate	12	Manufacturer

* As required in Project Documents and the QCP

- 5.4 **Process Control of Earthwork.** Include plans for control of gradation and moisture in stockpiles. Identify stockpiles by signing or other acceptable methods. Develop techniques for construction of proper stockpiles, loading, and spreading procedures to avoid segregation and control moisture. Create procedures to monitor and control compaction. List all sampling locations in the QCP. Determine Target Values, Action Limits and Suspension Limits for each tested material property.

A process is generally considered in control when test results are within the Action Limits. More restrictive criteria may be used in the QCP but a process is deemed out of control,

production suspended and corrective actions taken when:

- a) Two (2) points in a row fall outside the Suspension Limits, or
- b) Three (3) points in a row fall outside the Action Limits

Create stopping rules with corrective action plans particular to the project and quality control capabilities. Resume production and/or construction work only after resolution of corrective actions is completed. Identify the corrective actions on the applicable Control Chart(s).

5.5 **Sampling and Testing Frequencies** – Minimum for each material type.

- a) Gradation: One (1) test per 5,000 tons or 2,500 cubic yards
- b) Density: Two (2) tests per 5,000 tons or 2,500 cubic yards

Take gradation samples at the given frequency from the stock piles as well as at the placement location. Take density tests on the finished grade, reporting final results after compaction. On large fills of consistent materials sampling frequencies may be allowed decrease if the consistency is demonstrated to the Engineer. Sample and visually inspect for organic content in unclassified fills. If fill materials are too coarse to test, per project specifications, develop and monitor acceptable compaction methods.

Detail procedures for safely taking samples at the material source and on the grade for testing. Provide information on who, when, where and the sampling method. Include procedures to prevent contamination when transporting roadway samples.

5.6 **Additional QC Sampling and Testing.** Conduct additional tests as needed to ensure acceptance, particularly when:

- a) The material appears inconsistent with similar material being sampled
- b) The aggregate manufacture process or stockpile location is changed

5.7 **Gradation Control.** When applicable and 10 or more representative gradation test results from stock piles are available determine the arithmetic mean (\bar{x}) and standard deviation (s) from the formulas in ATM SP 7 for each sieve specified for acceptance of the given material. If the value of $\bar{x} \pm 2$ times s is within the specification bands (neglecting those over 100% or less than 0%) the material probably will meet project specifications.

Control gradations at the material source and on the grade at time of placement.

- a) Set the Target Value of each sieve at the arithmetic mean of representative tests.
- b) Set Action Limits at 2 times the standard deviation of the tests for each sieve above and below the target value and within the 0% and 100% boundaries.
- c) Set Suspension Limits at 3 times the standard deviation of the tests for each sieve above and below the target value also within the 0% and 100% boundaries.

Until enough test results are available suggest temporary Target Values, Action Limits and

Suspension Limits or:

- d) Use the center of the specification limits as the Target Value.
- e) Set the Action limits at the specification limits
- f) Set the Suspension limits at 1.5 times the percentage range between the Target Value and the Suspension limits within the 0% and 100% boundaries.

Plot the Target Value, Action Limits and Suspension Limits on Control Charts for each sieve as described in the General Requirements. Plot applicable test results on the control charts. As testing proceeds keep checking the new values of \bar{x} and s . Changes in these values may indicate need for corrective actions and/or changing the Target Value, Action Limits and Suspension Limits on Control Charts.

- 5.8 **Density Control.** Use nuclear density test gauges and procedures that are calibrated for the material being tested. When applicable create density control charts to present and monitor % compaction. When at least 10 representative density test results from on-grade testing of completed compaction are available determine the arithmetic mean (\bar{x}) and standard deviation (s) of the test results per the equations from ATM SP 7 on the given material samples. If the value of $\bar{x} - 2$ times s is within the specification limits the material probably will meet the project specifications.

Set up control charts to monitor density (reported as % Compaction) test results from the finished grade of each lift of each type of material. When acceptable results from the paragraph above are available, set up the control charts with the Target Value at \bar{x} , Action Limits at $\bar{x} - 2$ times s and Suspension Limits at $\bar{x} - 3$ times s .

Plot the Target Value, Action Limits and Suspension Limits on Control Charts for Compaction as described in the General Requirements. Plot test results from calibrated density gauges on grade on the control charts. As testing proceeds keep checking the new values of \bar{x} and s . Changes in these values may indicate need for corrective actions and/or changing the Target Value, Action Limits and Suspension Limits on Control Charts.

- 5.9 **Corrective Actions and Stopping Rules.** Provide Corrective Actions and Stopping Rules in the QCP for control of:

- a) Gradations of aggregates
- b) Moisture Content in the aggregates on grade
- c) Density/Compaction of finish-rolled lifts

6. Quality Control of Aggregate Base and Surface Course

6.1 **Introduction.** This section applies to Aggregate Base and Surface Course materials. Contractor Quality Control processes as stated herein are required on DOT&PF projects that have contract quantities for individual pay items equal to or greater than 20,000 tons or 10,000 cubic yards. Then perform all quality control testing necessary to control the production and construction processes in accordance with a QCP developed per these standard practices.

6.2 **Field Operating Procedures, Alaska Test Methods and Standard Practices** listed below are those used for materials acceptance and are thus recommended for QC. Some of these tests are for quality of the materials that must be checked prior to production. Other tests may be proposed in the QCP subject to the Engineer's review.

a) WAQTC Field Operating Procedures (FOPs)

- FOP for AASHTO T 2 Sampling of Aggregates
- FOP for AASHTO T 248 Reducing Samples of Aggregate to Testing Size
- FOP for AASHTO T 255/T 265 Moisture Content of Aggregate and Soil
- FOP for AASHTO T 27/T 11 Sieve Analysis of Aggregates and Soils
- FOP for AASHTO T 99/T 180 Moisture-Density Relations of Soils
- FOP for AASHTO T 85 Specific Gravity and Absorption of Coarse Aggregate
- FOP for AASHTO T 224 Correction for Coarse Particles in the Soil Compaction Test
- FOP for AASHTO T 89 Determining the Liquid Limit of Soils
- FOP for AASHTO 90 Determining the Plastic Limit and Plasticity Index of Soils
- FOP for AASHTO T 310 In-Place Density and Moisture Content of Soil and Soil-Aggregate by Nuclear Methods (Shallow Depth)

b) Alaska Test Methods (ATMs) and Standard Practices (SPs)

- ATM 203 Organic Content of Soils by Ignition
- SP 1 Terminology
- SP 2 Calibration of Mechanical Compaction Hammer/Rammer
- SP 4 Random Sampling
- SP 6 Rounding and Precision in Materials Test Reporting
- SP 7 Determination of Outlier Test Results

6.3 **Testing Equipment.** Provide a list of the testing equipment proposed for quality control testing, and the test methods and frequency of calibration or verification of the equipment in the QCP. Maintain a record of all equipment calibration or verification results at the testing facility. The maximum interval and procedures are in the Summary table in subsection 5.3.

6.4 **Process Control of Aggregate Base and Aggregate Surface Course.** Include plans for control of fracture, gradation and moisture in the stockpiles. Identify stockpiles by signing or other acceptable methods. Develop techniques for construction of proper stockpiles, loading and spreading procedures to avoid segregation and control moisture. Create procedures to monitor

and control compaction. List all sampling locations in the QCP. Determine Target Values, Action Limits and Suspension Limits for each tested material property.

A process is generally considered in control when test results are within the Action Limits. More restrictive limits may be used in the QCP but a process is deemed out of control, production suspended and corrective actions taken when:

- a) Two (2) points in a row fall outside the Suspension Limits, or
- b) Three (3) points in a row fall outside the Action Limits

Create stopping rules and corrective action plans particular to the project and quality control capabilities. Resume production and/or construction work only after resolution of corrective actions is completed. Identify the corrective actions on the applicable Control Chart(s).

6.5 **Sampling and Testing Frequencies** – Minimum for each material type

- a) Fracture: One (1) test per 1,000 tons or 500 cubic yards
- b) Gradation: One (1) test per 1,000 tons or 500 cubic yards
- c) Density: Two (2) tests per 1,000 tons or 500 cubic yards

Sample Fracture from stockpiles and on the grade at the frequency above keeping the test results separate. Take gradation samples at the given frequency from stock piles as well as at the placement location. Take density tests on the finished grade, reporting final results after compaction.

Detail procedures for safely taking samples at the material source and on the grade for testing. Provide information on who, when, where and the sampling method. Include procedures to prevent contamination when transporting roadway samples.

6.6 **Additional QC Sampling and Testing.** Conduct additional tests as needed to ensure acceptance, particularly when:

- a) The material appears inconsistent with similar material being sampled
- b) The aggregate manufacture process or stockpile location is changed

6.7 **Fracture Control.** When at least 10 representative fracture test results from stock piles for per FOP for AASHTO T 335 are available determine the arithmetic mean (\bar{x}) and standard deviation (s) of the test results per the equations from ATM SP 7 on the given material samples. If the value of $\bar{x} - 2$ times s is within the specification limits the material probably will meet the project specifications unless degradation occurs in the loading, hauling, placement and compaction operations.

Set up control charts for fracture test results from the stockpiles and on the grade. When acceptable results from the paragraph above are available, set up the control charts with the Target Value at \bar{x} , Action Limits at $\bar{x} - 2$ times s and Suspension Limits at $\bar{x} - 3$ times s .

Fracture tests are required for the first 20 samples at the start of production from any source. If the value of \bar{x} minus 2 times s of these tests is above the minimum fracture requirement the frequency for sampling and testing for fracture may be changed to one (1) test per 10,000 tons or 5,000 cubic yards.

- 6.8 **Gradation Control.** Control gradations of Aggregate Base and Surface Course as shown in Section 5.
- 6.9 **Density Control.** Control Density/Compaction of Aggregate Base and Surface Course as shown in Section 5.
- 6.10 **Corrective Actions and Stopping Rules.** Provide Corrective Actions and Stopping Rules in the QCP for control of:
 - a) Fracture of aggregates
 - b) Gradations of aggregates
 - c) Moisture Content in the aggregates on grade
 - d) Density/Compaction of finish-rolled lifts

7. Quality Control of Asphalt Treated Base Course

7.1 Introduction. This section applies to Asphalt Treated Base Course (ATB) materials composed of aggregates with hot asphalt cement as binder. Thus ATB is a Hot Mix Asphalt (HMA) with slightly modified QC requirements. Contractor Quality Control processes as stated herein are required on DOT&PF projects that have contract quantities for individual pay items equal to or greater than 5,000 tons of mix. When the above criteria are met perform all quality control testing necessary to control the production and construction processes in accordance with a QCP developed per these standard practices.

7.2 Field Operating Procedures, Alaska Test Methods and Standard Practices listed below are those used for materials acceptance and are thus recommended for QC. Some of these tests are for quality of the materials that must be checked prior to production. Other tests may be proposed in the QCP subject to the Engineer's review.

a) WAQTC Field Operating Procedures (FOPs)

- FOP for AASHTO T 2 Sampling of Aggregates
- FOP for AASHTO T 248 Reducing Samples of Aggregate to Testing Size
- FOP for AASHTO T 255 Moisture Content of Aggregate
- FOP for AASHTO T 27/T 11 Sieve Analysis of Aggregates and Soils
- FOP for AASHTO T 168 Sampling Bituminous Paving Mixtures
- FOP for AASHTO R 47 Reducing Samples of Hot Mix Asphalt to Testing Size
- WAQTC TM 11 Sampling Bituminous Material after Compaction (Obtaining Cores)
- FOP for AASHTO T 329 Moisture Content of Hot Mix Asphalt (HMA) by Oven Method
- FOP for AASHTO T 308 Determining the Asphalt Binder Content of Hot Mix Asphalt (HMA) By the Ignition Method. (For ATB with a Job Mix Formula)
- FOP for AASHTO T 209 Theoretic Maximum Specific Gravity and Density of Hot Mix Asphalt Paving Mixtures
- FOP for AASHTO TP 166/T 275 Bulk Specific Gravity and Percent Compaction of Hot Mix Asphalt
- WAQTC TM 8 In-Place Density of Bituminous Mixes Using the Nuclear Moisture-Density Gauge (for Density Control)
- FOP for AASHTO T 30 Mechanical Analysis of Extracted Aggregate

b) DOT&PF Alaska Test Methods and Standard Procedures

- ATM 403 Sampling Bituminous Mixes
- ATM 405 Asphalt Content of Hot Mix Asphalt by the Nuclear Method
- ATM 412 Standard Density by the Control Strip Method
- ATM 414 Anti-Strip Requirements of Hot Mix Asphalt
- SP 4 Random Sampling
- SP 6 Rounding and Precision in Materials Test Reporting
- SP 11 Contractor Quality Control

- 7.3 **Testing Equipment.** Include a list of the testing equipment proposed for quality control testing, and the test methods and frequency of calibration or verification of the equipment in the QCP. Maintain a record of all equipment calibration or verification results at the testing facility. Use the following maximum intervals and procedures:

SUMMARY OF EQUIPMENT REQUIRING CALIBRATION/VERIFICATION

Equipment *	Requirement	Max. Interval (Months)	Performed By:
Coarse Sieves (≥ #4 Sieve)	Check Openings and Physical Condition	6	Lab Personnel
Fine Sieves (< #4 Sieve)	Check Physical Condition	6	Lab Personnel
Test Thermometers	Standardize	6	Lab Personnel
Timers	Check Accuracy	6	Lab Personnel
Ovens	Verify Temperature Settings	4	Lab Personnel
Ignition Ovens	Verify Internal Balance	12	Lab Personnel
General Purpose Scales	Verify	12	Lab Personnel
Analytical Scales		12	
General Purpose Weights	Verify	12	Outside Agency
Analytical Weights		12	
Mechanical Shakers	Check Sieving Thoroughness	12	Lab Personnel
Length Measurement Devices	Standardize	12	Lab Personnel
Vacuum Systems	Check Critical Dimensions	12	Lab Personnel
Straight Edges	Check Plainness of Edge	6	Lab Personnel
Nuclear Density Gauges	Calibrate	12	Manufacturer

As Required in the Project Documents and the QCP

- 7.4 **Process Control of Asphalt Treated Base Course (HMA).** Include plans for control of fracture, gradation and moisture in the stockpiles. Develop techniques for construction of stockpiles to avoid segregation. Identify aggregate stockpiles by signing or other acceptable methods. Develop plant operation procedures to maintain target temperatures, gradation and asphalt content of the mixture. Develop loading, hauling and placement procedures to maintain proper temperatures and avoid segregation. Create procedures to

monitor and control compaction. List all sampling locations in the QCP. Determine Target Values, Action Limits and Suspension Limits for each tested material property.

A process is generally considered in control when test results are within the Action Limits. More restrictive limits may be used in the QCP but a process is deemed out of control, production stopped and corrective actions taken when:

- a) Two (2) points in a row fall outside the Suspension Limits, or
- b) Three (3) points in a row fall outside the Action Limits

Create stopping rules and corrective action plans particular to the project and quality control capabilities. Resume production and/or construction work after appropriate corrective actions are complete. Identify the corrective actions on the applicable Control Chart(s).

It is recommended to plot running averages of the test results after three tests are obtained. Running averages of tests computed for each lot may be helpful in maintaining quality of the mix.

7.5 Sampling and Testing Frequencies – Minimum. The sampling and testing frequencies pertain to production ATB materials. They are required in addition to any preliminary (source) material test requirements per the contract documents or private testing. Preliminary (source) testing results may be used to develop control charts for the production mix as long as they are representative of the same materials and use the same testing methods.

- a) Fracture: One (1) test per 500 tons produced
- b) Gradation: One (1) test per 500 tons
- c) Moisture Content of Aggregate: One (1) test with Gradation Sample
- d) Asphalt Cement Content: One (1) test per 500 tons of mixture
- e) Moisture Content of Mixture: Record with Asphalt Cement Content test results
- f) Density: Four (4) tests per 1,000 tons (record test results after finish rolling)
- g) Temperature of Asphalt Cement: Once per eight (8) hours of production (storage tank)
- h) Temperature of Mixture: Four (4) tests per 1,000 tons (behind the paver)

Detail procedures for safely taking samples at the plant and on the roadway for testing providing information on who, when, where and the sampling method. Include procedures to prevent contamination when transporting roadway samples.

7.6 Additional elements for the QCP are to include:

- a) Thickness, plans to monitor and control
- b) Segregation, plans to avoid mixture segregation as well as temperature segregation of the mix
- c) Smoothness, plans to monitor and control

7.7 Additional QC Testing will be needed when:

- a) The source aggregate is inconsistent with similar material being sampled
- b) The aggregate manufacture process or stockpile location is changed
- c) Asphalt Cement source changes

7.8 Fracture Control. Control Fracture of Asphalt Treated Base Course aggregates as shown in Section 6.

7.9 Gradation Control. When aggregate sampling prior to mixing is used control gradations of Asphalt Treated Base Course aggregates as shown in Section 5.

Record moisture contents with all gradation tests. Set corrective actions/stopping rules for possible level of moisture contents.

When Ignition Oven methods are used for gradation control and 10 or more representative gradation test results are available determine the arithmetic mean (\bar{x}) and standard deviation (s) from the formulas in ATM SP 7 for each sieve specified for acceptance of the given material. If the value of $\bar{x} \pm 2$ times s is within the specification bands (neglecting those over 100% or less than 0%) the material probably will meet project specifications.

- a) Set the Target Value of each sieve at the arithmetic mean of representative tests.
- b) Set Action Limits at 2 times the standard deviation of the tests for each sieve above and below the target value and within the 0% and 100% boundaries.
- c) Set Suspension Limits at 3 times the standard deviation of the tests for each sieve above and below the target value also within the 0% and 100% boundaries.

Until enough test results are available suggest temporary Target Values, Action Limits and Suspension Limits or:

- a) Use the center of the specification limits as the Target Value.
- b) Set the Action limits at the specification limits
- c) Set the Suspension limits at 1.5 times the percentage range between the Target Value and the Suspension limits within the 0% and 100% boundaries.

Plot the Target Value, Action Limits and Suspension Limits on Control Charts for each sieve as described in the General Requirements. Plot applicable test results on the control charts. As testing proceeds keep checking the new values of \bar{x} and s . Changes in these values may indicate need for corrective actions and/or changing the Target Value, Action Limits and Suspension Limits on Control Charts.

7.10 Asphalt Cement Content Control. When 10 or more representative asphalt cement content test results are available determine the arithmetic mean (\bar{x}) and standard

deviation (s) from the formulas in ATM SP 7 for the test results. If the value of $\bar{x} \pm 2$ times s is within the specification bands the material probably will meet project specifications.

- a) Set the Target Value of each sieve at the arithmetic mean of representative tests.
- b) Set Action Limits at 2 times the standard deviation of the tests for each sieve above and below the target value and within the 0% and 100% boundaries.
- c) Set Suspension Limits at 3 times the standard deviation of the tests for each sieve above and below the target value also within the 0% and 100% boundaries.

Until enough test results are available suggest temporary Target Values, Action Limits and Suspension Limits or:

- a) Use the center of the specification limits as the Target Value.
- b) Set the Action limits at the specification limits
- c) Set the Suspension limits at 1.5 times the percentage range between the Target Value and the Suspension limits

Plot the Target Value, Action Limits and Suspension Limits on Control Charts for each sieve as described in the General Requirements. Plot applicable test results on the control charts. As testing proceeds keep checking the new values of \bar{x} and s . Changes in these values may indicate need for corrective actions and/or changing the Target Value, Action Limits and Suspension Limits on Control Charts.

Record moisture contents with all gradation tests. Set corrective actions/stopping rules for possible level of moisture contents.

7.11 **Density Control.** Control Density of Asphalt Treated Base Course as shown in Section 5.

7.12 **Control of Temperature of Asphalt Cement.** Estimate a needed Target Value for asphalt binder temperature based on the required mixing temperature and typical plant operations specific to the mixture. Set up a control chart with that Target Value and plot the temperature test results. When 10 or more representative asphalt cement temperature test results are available determine the arithmetic mean (\bar{x}) and standard deviation (s) from the formulas in ATM SP 7 for the test results. If the \bar{x} value is near the estimated Target Value and/or the mix temperatures are acceptable:

- a) Set the Target Value of each sieve at the \bar{x} of representative tests.
- b) Set Action Limits at 2 times the standard deviation of the test results
- c) Set Suspension Limits at 3 times the standard deviation of the test results

If the \bar{x} is off the estimated Target Value and/or the mix temperatures are not acceptable as influenced by the asphalt cement temperatures take corrective actions to correct it.

Keep Control Charts as described in the General Requirements. Plot applicable test results on the control charts. As testing proceeds keep checking the new values of \bar{x} and s . Changes in these values may indicate need for corrective actions and/or changing the Target Value, Action Limits and Suspension Limits on Control Charts.

- 7.13 **Control of Temperature of Hot Mix Asphalt.** Estimate a needed Target Value for asphalt mix temperature needed at the plant and behind the screed of the paver (prior to compaction) based on the required compaction temperature and typical operations specific to the type of mixture. Set up control charts with that Target Values and plot the temperature test results. When 10 or more representative asphalt mix temperature tests results at the plant and from behind the screed are available determine the arithmetic mean (\bar{x}) and standard deviation (s) from the formulas in ATM SP 7 for the test results. If the \bar{x} value of the tests behind the screed is near the estimated Target Value and/or the mix temperatures are acceptable:

- a) Set the Target Value of the control charts at the \bar{x} of representative tests.
- b) Set Action Limits at 2 times the standard deviation on each side of the Target Values.
- c) Set Suspension Limits at 3 times the standard deviation on each side of the Target Values

If the \bar{x} is off the estimated Target Value and/or the hot mix asphalt temperatures are not acceptable take actions to correct it.

Keep Control Charts as described in the General Requirements. Plot applicable test results on the control charts. As testing proceeds keep checking the new values of \bar{x} and s . Changes in these values may indicate need for corrective actions and/or changing the Target Value, Action Limits and Suspension Limits on Control Charts.

- 7.14 **Control of ATB Thickness.** Include procedures for safely taking and recording thickness measurements of the loose mixture. Measure the HMA thicknesses immediately behind the paver screed and prior to compaction. Determine and show correlation between uncompacted and compacted thicknesses. The minimum frequency is one test for each hour of paving.

- 7.15 **Corrective Actions and Stopping Rules.** Provide Corrective Actions and Stopping Rules in the QCP for control of:

- a) Fracture of aggregates in the HMA
- b) Gradations of aggregates in the HMA
- c) Asphalt Cement Content in the HMA
- d) Density/Compaction of finish-rolled HMA
- e) Temperature of the Asphalt Cement
- f) Moisture of the aggregates at the plant

- g) Temperature of the mixture at the plant and behind the screed of the paver
- h) Moisture of the HMA on the roadway
- i) Thickness of HMA lifts

8. Quality Control of Hot Mix Asphalt

8.1 **Introduction.** This section applies to Hot Mix Asphalt (HMA) materials composed of aggregates using hot asphalt cement as binder. Contractor Quality Control processes as stated herein are required on DOT&PF projects that have contract quantities for individual pay items equal to or greater than 5,000 tons of any given type of HMA. When all the requirements stated above are met, perform all quality control testing necessary to control the production and construction processes in accordance with a QCP developed per these standard practices.

8.2 **Field Operating Procedures, Alaska Test Methods and Standard Practices:** See Section 7.2.

8.3 **Testing Equipment.** Use testing equipment for HMA as detailed in Section 7.

8.4 **Process Control of HMA.** Perform Process Control of HMA as detailed in Section 7.

8.5 **Sampling and Testing Frequencies – Minimum.** The sampling and testing frequencies pertain to production each type and lift of HMA materials. They are required in addition to any preliminary (source) material test requirements per the contract documents or private testing. Preliminary (source) testing results may be used to develop control charts for the production mix as long as they are representative of the same materials and use the same testing methods.

- a) Fracture: One (1) test per 250 tons produced
- b) Gradation: One (1) test per 250 tons
- c) Moisture Content of Aggregate: One (1) test with Gradation Sample
- d) Asphalt Cement Content: One (1) test per 250 tons of mixture
- e) Moisture Content of Mixture: Record with Asphalt Cement Content test results
- f) Density: One (1) test per 250 tons (record test results after finish rolling)
- g) Temperature of Asphalt Cement: In the storage tank, once per eight (8) hours of production
- h) Temperature of HMA: One (1) test per 250 tons (record test results behind the paver)

Detail procedures for safely taking samples at the plant and on the roadway for testing providing information on who, when and the method. Include procedures to prevent contamination when transporting roadway samples.

8.6 **Additional elements for the QCP to include:**

- a) Milling, when applicable

1. Milling Plan. The proposed general procedures for asphalt milling, and milled asphalt pavement materials removal.
 2. Equipment. The proposed equipment to mill or cut, and remove the existing materials. Include the make, model, serial number, manufactured year.
 3. Grade and Slope. The proposed procedure for measuring the grade and cross-slope of the finish surface of the milled roadway. Include the frequency of tests and equipment to be used.
- b) Balance operations. Explain the proposed methodology for balancing the operation, to include plant production, storage, transportation, placement, and compaction.
- c) Plant operations. The plant location, owner, producer name, and plant number and type that will be supplying the HMA mixture. Cite the number of bins feeding to the plant along with the material properties. Describe plans for loading and storage of HMA.
- d) Transportation of Mixtures. Minimum QCP procedures for transportation of HMA from the plant to the paver are as follows:
1. Truck Bed Covers. Cite criteria for when covers are to be used and the person responsible for directing the operations.
 2. Unloading. The procedures for truck unloading, and for removing the remaining mixture from the truck bed and bed apron.
 3. Transfer Vehicles. The type and size of Material Transfer Device or Windrow Elevators to be used and procedures for bridge crossings with the equipment.
- e) Paving. Minimum QCP procedures for placement of HMA are as follows:
1. Equipment. The Paver make, model, serial number, manufactured year, and documentation for the required retrofits.
 2. Paving Plan. The general sequence, the widths and depths of paving for each course(s) and the planned date for paving to begin and to be completed.
 3. Plan for obtaining and maintaining contract paving thicknesses
 4. Material Feed System. The procedure for processing the mixture through the paver.
 5. Grade and Slope. The procedure for controlling the grade and slope, including transition areas.
 6. Joints. The procedure for the construction of the longitudinal and transverse (supported and non-supported) joints. Include starting and stopping procedures for the paver for transverse joints.
 7. Compaction. The manufacturer's make, model, serial number, and manufactured year of all the equipment to be used in the compaction of the HMA. Include procedures for QC testing.
 8. Asphalt Materials. The source, source numbers, type and grade of materials to be used for the HMA, tack coat, prime coat, and construction joints.
 9. Control of Pavement Smoothness. Create a procedure for monitoring the profile of pavement to provide smoothness that meets allowable tolerances in the project specifications.

- 8.7 **Additional QC Testing will be needed when:**
- a) The source aggregate is inconsistent with similar material being sampled
 - b) The aggregate manufacture process or stockpile location is changed
 - c) Asphalt Cement source changes
- 8.8 **Fracture Control.** Control fracture of HMA aggregates as shown in Section 6.
- 8.9 **Gradation Control.** Control gradation of HMA aggregates as shown in Section 7.
- 8.10 **Asphalt Cement Content Control.** Control asphalt cement content of HMA as shown in Section 7.
- 8.11 **Density Control.** Control compaction of each HMA lift as shown in Section 5.
- 8.12 **Control of Temperature of Asphalt Cement.** Control the temperature of asphalt cement at the HMA plant as shown in Section 7.
- 8.13 **Control of Temperature of HMA.** Control the temperature of each HMA lift at the plant and behind the screed as shown in Section 7.
- 8.14 **Control of HMA Thickness.** Include procedures for taking and recording thickness measurements of the loose mixture. Measure the HMA thicknesses immediately behind the paver screed and prior to compaction. Determine and show correlation between uncompacted and compacted thickness. The minimum frequency is one test for each hour of paving.
- 8.15 **HMA Smoothness Control.** Provide procedures for monitoring, controlling and measuring the smoothness of the HMA course (surface, intermediate, and/or base) to obtain the best possible results.
- 8.16 **Corrective Actions and Stopping Rules.** Provide Corrective Actions and Stopping Rules in the QCP for control of:
- a) Fracture of aggregates in the HMA
 - b) Gradations of aggregates in the HMA
 - c) Asphalt Cement Content in the HMA
 - d) Density/Compaction of finish-rolled HMA
 - e) Temperature of the Asphalt Cement
 - f) Moisture of the aggregates at the plant
 - g) Temperature of the mixture at the plant and behind the screed of the paver
 - h) Moisture of the HMA on the roadway
 - i) Thickness of HMA lifts
 - j) Smoothness of completed HMA lifts

9. Quality Control of Portland Cement Concrete

9.1 **Introduction.** This section applies to Portland cement concrete (PCC) materials as shown in the project plans and specifications. Contractor Quality Control processes as stated herein are required on DOT&PF projects that have contract quantities for individual pay items equal to or greater than 500 cubic yards of any given class of PCC. When all the requirements stated above are met, perform all quality control testing necessary to control the production and construction processes in accordance with a QCP developed per these standard practices.

9.2 **Field Operating Procedures, Alaska Test Methods and Standard Practices** listed below are those used for materials acceptance and are thus recommended for QC. Some of these tests are for quality of the materials that must be checked prior to production. Other tests may be proposed in the QCP subject to the Engineer's review.

a) AASHTO Standards

- AASHTO T 231 Capping Cylindrical Concrete Specimens
- AASHTO T 22 Compressive Strength of Cylindrical Concrete Specimens
- AASHTO T 84 Specific Gravity and Absorption of Fine Aggregate

b) WAQTC Field Operating Procedures (FOPs):

- WAQTC TM 2 Sampling Freshly Mixed Concrete
- FOP for AASHTO T 309 Temperature of Freshly Mixed Concrete
- FOP for AASHTO T 119 Slump of Freshly Mixed Concrete
- FOP for AASHTO T 121 Density (Unit Weight), Yield & Air Content (Gravimetric) of Freshly Mixed Concrete
- FOP for AASHTO T 152 Air Content of Freshly Mixed Concrete by the Pressure Method
- FOP for AASHTO T 23 Making and Curing Test Specimens in the Field
- FOP for AASHTO T 85 Specific Gravity and Absorption of Coarse Aggregate

c) DOT&PF Alaska Test Methods and Standard Practices

- SP 4 Random Sampling
- SP 6 Rounding and Precision in Materials Test Reporting
- SP 8 Calibration of Pressure Type Air Meter
- SP 11 Contractor Quality Control

9.3 **Certification of Ready Mixed Concrete Production Facilities.** Provide a current National Ready Mix Concrete Association (NRMCA) Certificate of Conformance for Concrete Production Facilities along with a copy of the completed Check List and Forms used to obtain the Certificate. Obtain this Certificate in accordance with the latest version of the NRMCA's QC Manual Plant Certification Check List. A copy of the Plant

Certification Check List and other information concerning this certification may be obtained from the NRMCA at: 900 Spring Street, Silver Springs, MD 20910 or; Online at www.nrmca.org.

Plant Certification by the Plant Manager. Certification may be obtained by an inspection and evaluation conducted by the Plant Manager, defined as the person directly responsible for the daily plant operation, using and completing the NRMCA Plant Certification Check List. Correct all deficiencies to the satisfaction of the Plant Manager. The Plant Manager must sign the completed NRMCA Plant Certification Check List certifying all applicable items have been met. The certification by the Plant Manager is considered valid for 6 months from the date of inspection.

- 9.4 **Testing Equipment.** Include a list of the testing equipment proposed for quality control testing, and the test methods and frequency of calibration or verification of the equipment in the QCP. Maintain records of all equipment calibration or verification results at the testing facility. Use minimum frequency and procedures as shown in the Summary table below:

SUMMARY OF EQUIPMENT REQUIRING CALIBRATION/VERIFICATION

Equipment *	Requirement	Max. Interval (Months)	Performed By:
Coarse Sieves (\geq # 4 Sieve)	Check Openings and Physical Condition	6	Lab Personnel
Fine Sieves ($<$ #4 Sieve)	Check Physical Condition	6	Lab Personnel
Test Thermometers	Standardize	6	Lab Personnel
Timers	Check Accuracy	6	Lab Personnel
Ovens	Verify Temperature Settings	4	Lab Personnel
Compression Testing Machine	Verify Load Indications	12	Lab Personnel
General Purpose Scales	Verify	12	Lab Personnel
Analytical Scales		12	
General Purpose Weights	Verify	12	Outside Agency
Analytical Weights		12	
Mechanical Shakers	Check Sieving Thoroughness	12	Lab Personnel
Length Measurement Devices	Standardize	12	Lab Personnel
Slump Cones and Tamping Rods	Check Critical Dimensions	12	Lab Personnel
Straight Edges	Check Plainness of Edge	6	Lab Personnel
Single Use Molds	Check Dimensions	Each Shipment	Lab Personnel
Curing/Moist Room	Temperature Verified with Recording Thermometer	Continuous	Lab Personnel
	Check Recording Thermometer for Accuracy	6	
Air Meters	Calibrate	3	Lab Personnel
	Calibrate for Unit Weight	12	
Capping Material	Check Strength	3	Lab Personnel
Batching Scales	Verify Accuracy	6	Plant Personnel
Volumetric Batching Devices and Dispensers	Verify Accuracy	6	Plant Personnel
Devises for Automated Aggregate Moisture Measurement	Verify Accuracy	6	Plant Personnel

*As Required in the Project Documents and the QCP

9.5 **Process Control of PCC.** Include a plan for control of the aggregates stockpiles, identification of stockpiles by signing or other acceptable methods, techniques for construction of proper stockpiles, and loading procedures. Develop techniques for control of aggregate gradations, moisture content of aggregates, Slump, Air Content, Unit Weight, Water/Cement Ratio and Compressive Strength of concrete cylinders.

- a) Designate the procedures for sampling and testing the concrete mixture for slump, air content, unit weight, compressive strength and computing water/cement ratio.
 - 1. Start Slump, Air Content, Unit weight, and Water/Cement Ratio testing begins on the concrete mix from the first concrete truck for each day of production and if there is a change in production or method of delivery.
 - 2. Start Compressive Strength Sampling on other than the first concrete truck for each day of production. Test the two cylinders each and report the average at 7, 14, and 28 days

Estimate a needed Target Values for applicable material properties based on the mix design and typical operations specific to the mixture. Set up a control chart with that Target Value and plot the test results. When 10 or more representative asphalt cement temperature test results are available determine the arithmetic mean (\bar{x}) and standard deviation (s) from the formulas in ATM SP 7 for the test results. If the \bar{x} value is near the estimated Target Value and/or the properties generally are acceptable:

- a) Set the Target Value of each sieve at the \bar{x} of representative tests.
- b) Set Action Limits at 2 times the standard deviation of the test results
- c) Set Suspension Limits at 3 times the standard deviation of the test results

If the \bar{x} is off the estimated Target Value and/or the materials generally are not acceptable Take corrective actions as defined in the QCP or as directed by the PA to correct the problem.

Keep Control Charts as described in the General Requirements. Plot applicable test results on the control charts. As testing proceeds keep checking the new values of \bar{x} and s . Changes in these values may indicate need for corrective actions and/or changing the Target Value, Action Limits and Suspension Limits on Control Charts.

A process is generally considered in control when test results are within the Action Limits. More restrictive limits may be used in the QCP but a process is deemed out of control, production stopped and corrective actions taken when:

- a) Two (2) points in a row fall outside the Suspension Limits, or
- b) Three (3) points in a row fall outside the Action Limits

Create stopping rules and corrective action plans particular to the project and quality

control capabilities. Resume production and/or construction work after appropriate corrective actions are complete. Identify the corrective actions on the applicable Control Chart(s).

9.6 Sampling and Testing Frequencies – Minimum

- a) Gradation (Fine and Coarse Aggregates): One (1) test per 50 cubic yards (plant)
- b) Moisture Content of Aggregates (Fine and Coarse Aggregates): One (1) in each per day of production
- c) Slump: One (1) test per 25 cubic yards (plant)
- d) Slump: One (1) test per 25 cubic yards (site)
- e) Air Content: One (1) test per 25 cubic yards (plant)
- f) Air Content: One (1) test per 25 cubic yards (site)
- g) Unit Weight: One (1) test per 25 cubic yards (plant)
- h) Unit Weight: One (1) test per 25 cubic yards (site)
- i) Water /Cement Ratio: One (1) per truck (plant)
- j) Water /Cement Ratio: One (1) per 100 cubic yards (site)
- k) Compressive Strength: One set of six (6) cylinders per 25 cubic yards (site). Non-structural and minor concrete construction requires only one set of cylinders.

When placing deck concrete that is 80°F or hotter, install equipment at the site to measure relative humidity and wind velocity. Monitor the surface evaporation rate of the concrete per the charts given in the project specifications. React to results per the project requirements.

9.7 Additional elements for the QCP to include:

- a) Process Control of the Aggregates. Describe procedures for monitoring aggregate gradation, water absorption and Saturated Surface Dry (SSD) Bulk Specific Gravity to verify compliance with the properties of the aggregates.
- b) Concrete Batching. The techniques and controls of the concrete batching operations. A description of the general operation, batching system, including the capacity, intended batch size, recording and the methods and sequence by which the plant produces a batch. Report initial and routine equipment checks, including those performed on the scales, water meters, admixture dispensers, mixing equipment, and agitators, if applicable. Include all material checks along with frequencies of testing.
- c) Process Control of Reinforcing Steel. Set up a frequency and procedures for monitoring and maintaining the required depth of concrete over the uppermost bar of the top mat of reinforcing steel. Obtain measurements as soon as the concrete is placed and struck off while it is still plastic.
- d) Response to Test Results. Provide responses to process control testing that include at least the following:
 - 1. Water Absorption. The procedure for corrective action when the absorption test results differ from the mixture design value by more than 0.5 percent.

2. Bulk Specific Gravity (SSD). The procedure of corrective action when the bulk specific gravity (SSD) of fine aggregate differs from the mixture design value by more than 0.056 or the bulk specific gravity (SSD) of coarse aggregate differs from the mixture design value by more than 0.032.
 3. Unit Weight. The procedure for corrective action when the measured unit weight is not within process control limits from the value established by the measured air content and the linear equation representing the concrete mix design. Use process control limits not exceeding $\pm 1.0 \text{ lb/ft}^3$ (16 kg/m^3) from the target value.
 4. Slump. The procedure for corrective action when the slump is not within process control limits. Establish process control limits from a target slump to ensure that the concrete is within the concrete mix criteria at the point of placement.
 5. Air Content. The procedure for corrective action when the air content is not within process control limits. Establish process control limits from the target value, to ensure that the concrete produced is within the specification limits.
 6. Other Quality Control Tests. The procedure for corrective action for test results outside of satisfactory limits established for each type of test.
- e) Concrete Hauling. Plan the equipment and methods for delivery of the concrete. Provide a description or plan drawing of the haul route for delivery of the concrete mix to the site of work. The patterns may be adjusted for unanticipated conditions without an addendum to the QCP.
 - f) Concrete Placement. Provide procedures for placement of the concrete to include as a minimum the placing sequence, identification of the placing equipment, and a description of the pumping procedures, if applicable.
 - g) Concrete Finishing, Texturing and Curing. List the methods for finishing, texturing, and curing concrete. Include the description and identification of equipment.

9.8 **Materials.** The source, transportation, handling, and storage procedures, for:

- a) Admixtures – type
- b) Aggregates – sizes
- c) Curing Materials
- d) Reinforcing Steel – size and type
- e) Portland Cement – type
- f) Water – potable or non-potable. If non-potable, the sampling and testing procedures shall be included.

10. Definitions of Terms and Acronyms

AASHTO – American Association of State Highway and Transportation Officials. This organization publishes test methods and specifications annually. The current version applies here.

ACI – American Concrete Institute

ASTM – American Society of Testing and Materials. This organization publishes test methods and specifications annually. The current version applies here.

ATM – Alaska Test Methods that are a compilation of materials Test Methods that are approved by the FHWA and FAA for use on Alaska Department of Transportation and Public Facilities projects.

DOT&PF – Alaska Department of Transportation and Public Facilities.

QA - Quality assurance: (1) All those planned and systematic actions necessary to provide confidence that a product or facility will perform satisfactorily in service; or (2) making sure the quality of a product is what it should be. [QA addresses the overall process of obtaining the quality of a service, product, or facility in the most efficient, economical, and satisfactory manner possible. Within this broad context, QA includes the elements of quality control, independent assurance, acceptance, dispute resolution etc. The use of the term QA/QC or QC/QA is discouraged and the term QA should be used. QA involves continued evaluation of the activities of planning, design, development of plans and specifications, advertising and awarding of contracts, construction, and maintenance, and the interactions of these activities.]

QC - Quality control - also called *process control*. The system used by a contractor to monitor, assess and adjust their production or placement processes to ensure that the final product will meet the specified level of quality. Quality control includes sampling, testing, inspection and corrective action (where required) to maintain continuous control of a production or placement process.

QC/QC – See QA.

QCO – Quality Control Organization. This is the Contractor's organization for smooth and safe operation of the QCP including the Plan Administrator and Quality Control Technicians.

QCP – Stands for the Contractor's Quality Control Plan that is developed specifically for a project.

PA – Stands for the Contractor's Plan Administrator of the QCP.

Process Control – See QC.

WAQTC – Stands for Western Alliance for Quality in Transportation Construction. This organization of western states publishes FOP's for AASHTO test methods to clarify their use in the field of acceptance and quality control. This organization also develops and provides training for qualification of technicians who perform the tests

This page intentionally left blank.